


VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program


Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130291 ✓			
Name	Sean Fielding	ID#	5189	Date	3/14/08	
A	Agency	Denali National Park		Phone #	683 9528	
	Instrument Location	Denali National Park - HQ				
B	Alco S/N	78259 ✓	Target Value	.086 ✓	High Pressure	500
	Alco Test Value Average	.079	.079			
		1 st Alco	2 nd Alco			
Signature			 3/15/08			
(OVER)						

Under the Alaska Rules of Evidence, I certify that:
(Do Not Write in the area below)


(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Sean Fielding, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

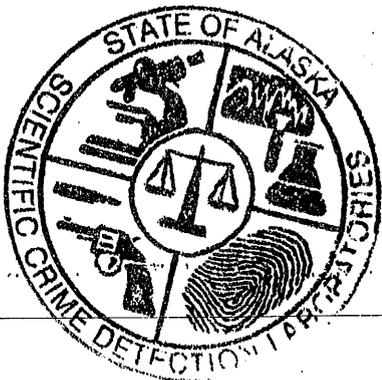

Signed and sealed,



Jeanne Swartz
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

3/24/08
Date

MAR 19 2008

VERIFICATION OF CALIBRATION REPORT

of DataMaster edm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster edm S/N 130291

(CONTINUED FROM FRONT PAGE)

C. TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER edm 130291

MARCH 14, 2008

OPERATOR'S NAME: *COB 3/24/08*
FIELDING/SEAN/R
OPERATOR'S NUMBER: 5189
SUBJECT'S LAST NAME:
VERIFICATION OF CAL
SUBJECT'S FIRST NAME/MI:

A
O.L. #: 1234567
DEPT/AGENCY: DNLB
CASE/REPORT: 031400
TEST TYPE: V
ALCO TARGET VALUE: .006
ALCO S/N: 78259

--- BREATH ANALYSIS ---

20/15/08

.006 ADJUSTED FOR 28.13 in		
ALCO TARGET	.000	15:37
BLANK TEST	.000	15:38
INTERNAL STANDARD	VERIFIED	15:38
ALCO TV 28.13 in	.079	15:38
BLANK TEST	.000	15:39
SUBJECT SAMPLE	.006	15:39
BLANK TEST	.000	15:40
ALCO TV 28.13 in	.079	15:40
BLANK TEST	.000	15:41

COB 3/24/08

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER edm 130291

MARCH 14, 2008
TIME 15:34

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 02/20/01
HEATERS
SAMPLE CHAMBER: 49c
BREATH TUBE: 41c
BAROMETER: 28.13 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

!@#%&'()*+,-./0123456789:;<=>?@ABCDEF
HIJKLMNOPQRSTUVWXYZ[\]^_`abcdefgijklmnop
qrstuvwxyz{|}~`