


VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

APR 28 2010

State of Alaska


Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130291
Name	Sean Fielding	ID#	5289
		Date	4/23/10
A	Agency	Denali National Park	Phone # 683 9528
	Instrument Location	Denali National Park - HQ	
Alco S/N		x301533	Target Value .083
			High Pressure 500
B	Alco Test Value Average	.085	.085
		1 st Alco	2 nd Alco
Signature			
		(OVER)	

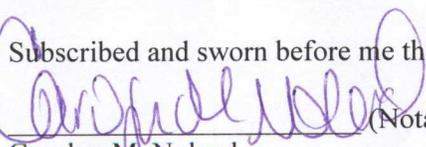
MSB
5/3/10

I, Nita J. Bolz, after being first duly sworn, depose and state as follows: (Do Not write in the area below)

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 18th day of June, 2010.


(Notary Seal Stamp)
Carolyn M. Noland
Notary Public, State of Alaska
Commission Expires with Office



VERIFICATION OF CALIBRATION REPORT

0105 6 5 89A

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130291

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130291

APRIL 23, 2010

OPERATOR'S NAME:
FIELDING/SEAN/R
OPERATOR'S NUMBER: 5189
SUBJECT'S LAST NAME:
VERIFICATION OF CAL
SUBJECT'S FIRST NAME/MI :

A
O.L. #: 1234567
DEPT/AGENCY: DNL8
CASE/REPORT: 042310
TEST TYPE: U

ALCO TARGET VALUE: .083
ALCO S/N: X01553

--- BREATH ANALYSIS ---

.083 ADJUSTED FOR 28.04 in

ALCO TARGET	.077	14:39
BLANK TEST	.000	14:40
INTERVAL STANDARD	VERIFIED	14:40
ALCO TU 28.04 in	.085	14:40
BLANK TEST	.000	14:41
SUBJECT SAMPLE	.000	14:41
BLANK TEST	.000	14:42
ALCO TU 28.04 in	.085	14:43
BLANK TEST	.000	14:43

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130291

APRIL 23, 2010
TIME 14:48

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 02/20/01
HEATERS
SAMPLE CHAMBER: 49c
BREATH TUBE: 42c
BAROMETER: 28.04 in
PUMP DETECTOR: OKAY

PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

!"#\$%&'()*+,-./0123456789:;<=>?@ABCDEFGHIJ
KLMNOPQRSTUVWXYZ[\]^_`abcdefgijklmnop
qrstuvwxyz{|}~■