



VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130291
A	Name	Sean Fielding	ID# 5789 - Date 6/6/08 ✓
	Agency	Denali National Park	Phone # 688-9528
	Instrument Location	Denali National Park - H	
B	Alco S/N	78259 ✓	Target Value .086 ✓ High Pressure 500
	Alco Test Value Average	.079 1 st Alco	.078 2 nd Alco
	Signature		 6/20/08


(OVER)

Under the Alaska Rules of Evidence, I certify that;
(Do Not write in the area below)


(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Sean Fielding, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

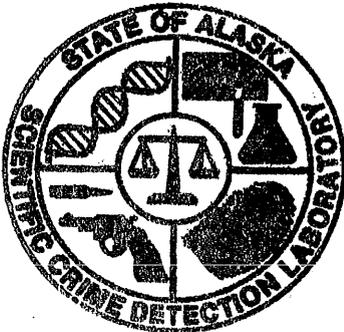

Signed and sealed,



6/20/08

Jeanne Swartz
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

Date

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130291

(CONTINUED FROM FRONT PAGE)

C. TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130291

JUNE 06, 2008

OPERATOR'S NAME:
FIELDING/SEAN/R
OPERATOR'S NUMBER: 5199
SUBJECT'S LAST NAME:
VERIFICATION OF CAL.
SUBJECT'S FIRST NAME/MI:

A
O.L. #: 1234567
DEPT/AGENCY: DMLB
CASE/REPORT: 060508
TEST TYPE: V
ALCO TARGET VALUE: .086 ✓
ALCO S/N: 78259 ✓

--- BREATH ANALYSIS ---

.086 ADJUSTED FOR 27.78 in
ALCO TARGET .079 09:43
BLANK TEST .000 09:45
INTERNAL STANDARD VERIFIED 09:45
ALCO TV 27.80 in .079 ✓ 09:45
BLANK TEST .000 09:46
SUBJECT SAMPLE .086 09:47
BLANK TEST .000 09:47
ALCO TV 27.78 in .078 09:48
BLANK TEST .000 09:48

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130291

JUNE 06, 2008 ✓
TIME 09:55

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 02/20/01
HEATERS
SAMPLE CHAMBER: 43c
BREATH TUBE: 43c
BAROMETER: 27.80 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

"#%&'()*+,-./0123456789:;<=>@ABCDEFGHIJKL
MNOPQRSTUVWXYZ . , ' " : ; < > [\] ^ _ ` { | } ~
!@#\$%^&*~