

JAN 06 <sup>2011</sup>~~2010~~ <sub>5/9/11</sub>

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	<u>130292</u> ✓
Name	<u>TRACY MORPHY</u>	ID#	<u>7152</u> ✓
		Date	<u>1-3-2011</u> ✓
A	Agency	<u>JUNEAU POLICE DEPT</u>	Phone # <u>907-582-0600</u>
	Instrument Location	<u>JUNEAU POLICE DEPT</u>	
B	Alco S/N	<u>X172933</u> ✓	Target Value <u>0.078</u> ✓
		High Pressure	<u>30.01</u>
	Alco Test Values	<u>0.082</u> ✓ 1st Alco	<u>0.081</u> ✓ 2 <sup>nd</sup> Alco
	Signature		


(OVER)

*BMB*  
*2/8/11*

(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:


- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

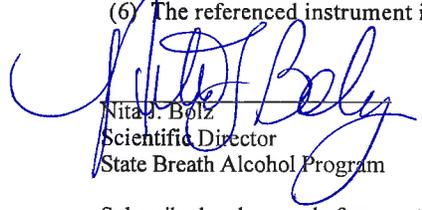  
 Nita J. Bolz  
 Scientific Director  
 State Breath Alcohol Program

Subscribed and sworn before me this 10<sup>th</sup> day of MAR, 2011

 (Notary Seal Stamp)

Daniel L. Nicholas  
Notary Public, State of Alaska  
Commission Expires with Office

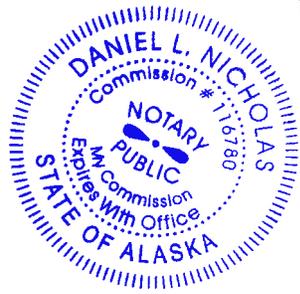

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska


Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130292

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

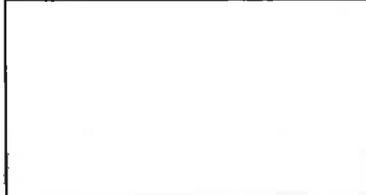

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130292

JANUARY 03, 2011

OPERATOR'S NAME:

MURPHY/TRACY/ERNEST

OPERATOR'S NUMBER: 7252

SUBJECT'S LAST NAME:

MURPHY

SUBJECT'S FIRST NAME/MI :

TRACY/E

O.L. #: VOC

DEPT/AGENCY: JNU1

CASE/REPORT: VOC

TEST TYPE: V

ALCO TARGET VALUE: .078

ALCO S/N: X172933

--- BREATH ANALYSIS ---

.078 ADJUSTED FOR 30.01 in  
ALCO TARGET .078 18:11  
BLANK TEST .000 18:12  
INTERNAL STANDARD VERIFIED 18:12  
ALCO TV 30.01 in .082 18:12  
BLANK TEST .000 18:13  
SUBJECT SAMPLE .000 18:13  
BLANK TEST .000 18:14  
ALCO TV 30.01 in .081 18:14  
BLANK TEST .000 18:15

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130292

JANUARY 03, 2011

TIME 18:08

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 01/08/09  
HEATERS  
SAMPLE CHAMBER: 49c  
BREATH TUBE: 42c  
BAROMETER: 30.01 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

PRINTER TEST

!"#\$%&'()\*+,-./0123456789:;<=>?@ABCDEFGHIJKL  
MNOPQRSTUVWXYZ[\]^\_`abcdefghijklmnopqr  
stuvwxyz{|}~\*~