

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument


State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N <u>130292</u> ✓	
Supervisor/Operator Performing the Verification Procedure:	
Name <u>Sergeant John Wahl</u> ✓	ID# <u>6393</u> Date <u>08/15/08</u> ✓
A Agency <u>Haines Borough Police Department</u> ✓	Phone # <u>766-2121</u>
Instrument Location <u>Haines Rural Jail Facility</u>	
Alco S/N <u>57324</u> ✓	Target Value <u>.080</u> ✓ High Pressure <u>400</u>
Alco Test Value Average <u>.081</u> ✓	<u>.079</u> ✓
1 st Alco	2 nd Alco
Signature <u>SGT John Wahl #216</u>	<u>CAS</u> <u>8/21/08</u>
(OVER)	

Under the Alaska Rules of Evidence, I certify that, (Do Not write in the area below)

- (a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.
- (b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, John Wahl, whose name appears in my records, is qualified to verify the calibration of the above instrument.
- (c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

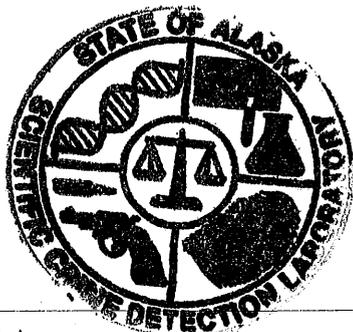

Signed and sealed,

Jeanne Swartz 8/25/08
Jeanne Swartz Date
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

AUG 21 2008

~~AUG 19 2008~~

CW
8/21/08

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130292 ✓

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130292

AUGUST 15, 2008 ✓

OPERATOR'S NAME: WAHL, JOHN A
OPERATOR'S NUMBER: 6393
SUBJECT'S LAST NAME:
VERIFICATION OF CAL
SUBJECT'S FIRST NAME/MI: N/A
O.L. #: N/A
DEPT/AGENCY: HNS1
CASE/REPORT: N/A
TEST TYPE: V
ALCO TARGET VALUE: .080 ✓
ALCO S/N: 57324 ✓

--- BREATH ANALYSIS ---

.080 ADJUSTED FOR 30.25 in
ALCO TARGET .080 18:42
BLANK TEST .000 18:43
INTERNAL STANDARD VERIFIED 18:43
ALCO TO 30.25 in .081 ✓ 18:44
BLANK TEST .000 18:44
SUBJECT SAMPLE .080 ✓ 18:45
BLANK TEST .000 18:46
ALCO TO 30.25 in .079 ✓ 18:46
BLANK TEST .000 18:47

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130292

AUGUST 15, 2008 ✓
TIME 18:38

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 02/20/01
HEATERS
SAMPLE CHAMBER: 49c
BREATH TUBE: 41c
BAROMETER: 30.25 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

!"#\$%&'()*+,-./0123456789:;{<=>?@ABCDEFGHIJ
KLMNOPQRSTUVWXYZ[\]^_`abcde fghijklmno
pqrstuvwxyz{|}~