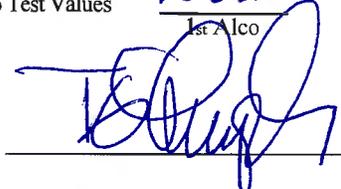


DEC 29 2010

# VERIFICATION OF CALIBRATION REPORT

*of DataMaster cdm Breath Test Instrument  
State of Alaska*

*Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program*


Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N <u>130292</u> ✓
Name	<u>TRACY MURPHY</u>	ID# <u>7252</u> ✓ Date <u>12-2-10</u> ✓
A Agency	<u>JUNEAU POLICE DEPT</u> Phone # <u>907.586-0600</u>	
Instrument Location	<u>JUNEAU POLICE DEPT</u>	
B Alco S/N	<u>X172933</u> ✓	Target Value <u>.078</u> ✓ High Pressure <u>30.35</u>
Alco Test Values	<u>.082</u> ✓ 1st Alco	<u>.082</u> ✓ 2 <sup>nd</sup> Alco
Signature		<u>008</u> 12/30/10

(OVER)

(Do Not write in the area below)


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

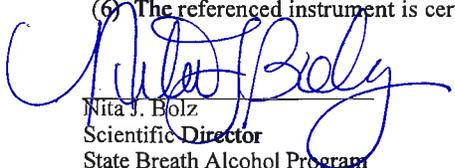  
 Nita J. Bolz  
 Scientific Director  
 State Breath Alcohol Program

Subscribed and sworn before me this 18<sup>th</sup> day of JAN 2011 2010-01-18

  
 (Notary Seal Stamp)  
 Daniel L. Nicholas  
 Notary Public, State of Alaska  
 Commission Expires with Office

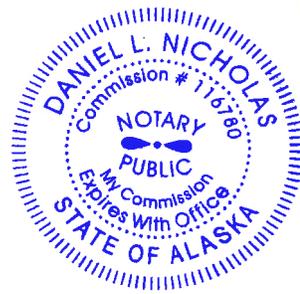

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument  
State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130292

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130292

DECEMBER 02, 2010

OPERATOR'S NAME:  
MURPHY/TRACY/ERNEST  
OPERATOR'S NUMBER: 7252  
SUBJECT'S LAST NAME:  
MURPHY  
SUBJECT'S FIRST NAME/MI :  
TRACY

O.L. #: VOC  
DEPT/AGENCY: JNU1  
CASE/REPORT: VOC  
TEST TYPE: V  
ALCO TARGET VALUE: .078  
ALCO S/N: X172933

--- BREATH ANALYSIS ---

.078 ADJUSTED FOR 30.37 in  
ALCO TARGET .079 15:55  
BLANK TEST .000 15:56  
INTERNAL STANDARD VERIFIED 15:56  
ALCO TV 30.37 in .082 15:57  
BLANK TEST .000 15:57  
SUBJECT SAMPLE .000 15:58  
BLANK TEST .000 15:59  
ALCO TV 30.37 in .082 15:59  
BLANK TEST .000 16:00

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130292

DECEMBER 02, 2010  
TIME 15:52

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 01/08/09  
HEATERS  
SAMPLE CHAMBER: 48c  
BREATH TUBE: 42c  
BAROMETER: 30.35 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY