

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:	
Name <u>D.R. STURKIE</u>	DataMaster cdm S/N <u>130293</u> ✓
ID# <u>3559</u> ✓	Date <u>9-1-10</u> ✓
A Agency <u>Anchorage Police Dept.</u>	Phone # <u>786-8900</u>
Instrument Location <u>Eagle River Substation (APD)</u>	
B Alco S/N <u>75260</u> ✓ Target Value <u>.081</u> ✓ High Pressure <u>900</u>	
Alco Test Values	<u>.079</u> ✓ 1st Alco
	<u>.080</u> ✓ 2nd Alco
Signature	<u>[Signature]</u>

(OVER)

*[Handwritten initials]*  
9/3/10


(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:


- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

[Signature]  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 9th day of Nov, 2010.

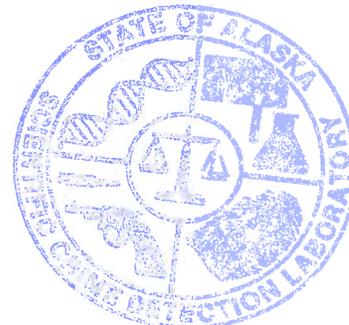

[Signature] (Notary Seal Stamp)  
Daniel L. Nicholas  
Notary Public, State of Alaska  
Commission Expires with Office



# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N

130293 9/3/10

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130293

SEPTEMBER 01, 2010

OPERATOR'S NAME: STURKIE  
OPERATOR'S NUMBER: 3559  
SUBJECT'S LAST NAME: UOC

SUBJECT'S FIRST NAME/NI :

L

O.L. #: L

DEPT/AGENCY: ANCI

CASE/REPORT: L

TEST TYPE: U

ALCO TARGET VALUE: .001

ALCO S/N: 75260

### --- BREATH ANALYSIS ---

.001 ADJUSTED FOR 29.68 in  
ALCO TARGET .000 03:04  
BLANK TEST .000 03:05  
INTERNAL STANDARD VERIFIED 03:05  
ALCO TV 29.68 in .079 03:06  
BLANK TEST .000 03:06  
SUBJECT SAMPLE .000 03:07  
BLANK TEST .000 03:07  
ALCO TV 29.68 in .000 03:08  
BLANK TEST .000 03:08

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130293

SEPTEMBER 01, 2010  
TIME 03:10

### --- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 01/08/09  
HEATERS  
SAMPLE CHAMBER: 50c  
BREATH TUBE: 48c  
BAROMETER: 29.68 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

### PRINTER TEST

!"#\$%&'()\*+,-./0123456789:;<=>?@ABCDEFGHIJKL  
MNPQRSTUVWXYZ[\]^\_`abcdefgijklmnop  
qrstuvwxyz{|}~