

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130294 ✓
A	Name	Michael Potter	ID# 5841 Date 7-22-08 ✓
	Agency	AST / AWT	Phone # 856-1634
	Instrument Location	Galena ✓	
B	Alco S/N	77675 ✓	Target Value .076 ✓ High Pressure 100
	Alco Test Value Average	.075 ✓ 1 st Alco	.075 ✓ 2 nd Alco
	Signature	<i>Michael Potter</i>	COB 7/29/08


(OVER)

Under the Alaska Rules of Evidence, I certify that (Identify that) the area below)

(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Michael Potter, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

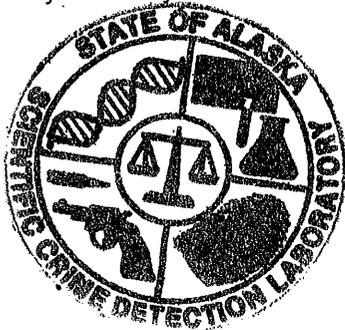

Signed and sealed,

Jeanne Swartz

Jeanne Swartz
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

7/30/08
Date

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130294

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130294

JULY 22, 2008

OPERATOR'S NAME:
FOTTER/MICHAEL/J
OPERATOR'S NUMBER: 5041
SUBJECT'S LAST NAME:
CAL VERIFICATION
SUBJECT'S FIRST NAME/NI :
Q

O.L. #: Q
DEPT/AGENCY: 6AL1
CASE/REPORT: Q
TEST TYPE: V
ALCO TARGET VALUE: .076 ✓
ALCO S/N: 77675 ✓

--- BREATH ANALYSIS ---

.076 ADJUSTED FOR 29.85 in		
ALCO TARGET	.075	14:36
BLANK TEST	.000	14:36
INTERNAL STANDARD	VERIFIED	14:37
ALCO TV 29.85 in	.075 ✓	14:37
BLANK TEST	.000	14:38
SUBJECT SAMPLE	.000	14:38
BLANK TEST	.000	14:39
ALCO TV 29.85 in	.075	14:39
BLANK TEST	.000	14:40

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130294

JULY 22, 2008 ✓
TIME 14:41

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 02/20/01
HEATERS
SAMPLE CHAMBER: 40c
BREATH TUBE: 42c
BAROMETER: 29.85 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

! " # % & ' () * + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G
H I J K L M N O P Q R S T U V W X Y Z [\] ^ _ ` a b c d e f g h i j k l m n o
p q r s t u v w x y z { | } ~ #