

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument
State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N: 130295

Supervisor / Operator Performing the Verification Procedure:

Name: William A. Mills ID#: 2688 Date: March 04, 2008


A. Agency: Hoonah Police Department Phone #: 945-3655

Instrument Location: 379 Raven Drive, Hoonah

Alco S/N: X124669 ✓ Target Value: .083 ✓ High Pressure: 800 psi

B. Alco Test Value Average: .082 .082
1st Alco 2nd Alco

Signature

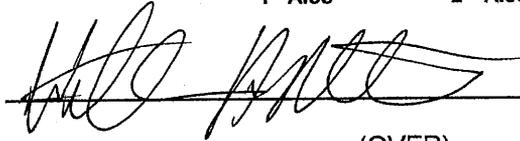

(OVER)

COB
3/18/08


Under the Alaska Rules of Evidence, I certify that:

(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, William Mills, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.


Signed and sealed,



Jeanne Swartz
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

Date

3/18/08

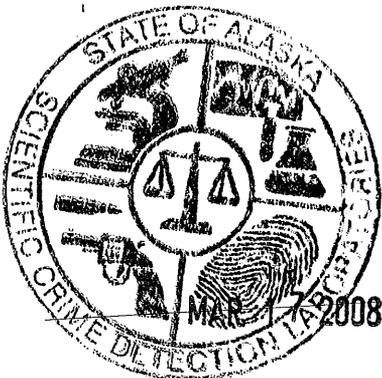

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130295

MARCH 04, 2008

COB 3/18/08
OPERATOR'S NAME:
MILLS WILLIAM A
OPERATOR'S NUMBER: 2688
SUBJECT'S LAST NAME:
VERIFICATION OF
SUBJECT'S FIRST NAME/MI :
CALIBRATION
O.L. #: 1234567890
DEPT/AGENCY: HNH1
CASE/REPORT: 1234567890
TEST TYPE: U
ALCO TARGET VALUE: .003
ALCO S/N: X124669

--- BREATH ANALYSIS ---

.003 ADJUSTED FOR 30.58 in
ALCO TARGET .004 22:45
BLANK TEST .000 22:46
INTERNAL STANDARD VERIFIED 22:46
ALCO TU 30.58 in .002 22:46
BLANK TEST .000 22:47
SUBJECT SAMPLE .000 *COB 3/18/08* 22:48
BLANK TEST .000 22:49
ALCO TU 30.58 in .002 22:49
BLANK TEST .000 22:50

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130295

MARCH 04, 2008
TIME 22:52

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 02/20/01
HEATERS
SAMPLE CHAMBER: 48c
BREATH TUBE: 42c
BAROMETER: 30.58 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

! " # \$ % & ' () * + , - . / 0 1 2 3 4 5 6 7 8 9 : ; (=) ? @ A B C D E F G
H I J K L M N O P Q R S T U V W X Y Z [\] ^ _ ` a b c d e f g h i j k l m n o
p q r s t u v w x y z { | } ~ #

80:81'E

ENTWY