

VERIFICATION OF CALIBRATION REPORT

Of Data-Master cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory -- Statewide Breath Alcohol Program

DEC 16 2010

Data-Master cdm S/N: 130296 ✓

Supervisor/Operator Performing the Verification Procedure:

Name John J. Waldron ID: # 3392 ✓ Date: 12/04/10 ✓


A. Agency Unalaska Department of Public Safety Phone 907-581-1233

Instrument Location Unalaska Department of Public Safety, PO Box 370, 29 Safety Way, Unalaska, AK 99685

Alco S/N: 78966 ✓ Target Value: .082 ✓ High Pressure: 400

B. Alco Test Values

	<u>.083</u> ✓ 1 st Test Value	<u>.083</u> ✓ 2 nd Test Value
--	---	---

Signature 

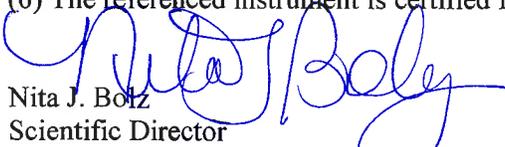
(OVER)

BMB
12/12/10

(Do not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

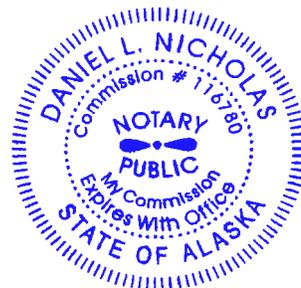
- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 18th day of JAN, 2011 *DN*

(Notary Seal Stamp)

Daniel L. Nicholas
Notary Public, State of Alaska
Commission Expires with Office



VERIFICATION OF CALIBRATION REPORT
Of Data-Master cdm Breath Test Instrument
State of Alaska
Scientific Crime Detection Laboratory -- Statewide Breath Alcohol Program

Data-Master cdm S/N: 130296

Supervisor/Operator & Number Performing the Verification Procedure: John J. Waldron, #3392
 Department and Date: Unalaska DPS,

(CONTINUED FROM FRONT PAGE)

C. TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
 DATAMASTER cdm 130296

DECEMBER 04, 2010 *AWB 12/23/10*

OPERATOR'S NAME: *AWB*
 WALDRON/JOHN/J

OPERATOR'S NUMBER: 3392

SUBJECT'S LAST NAME:
 UOC

SUBJECT'S FIRST NAME/MI :
 UOC

O.L. #: 0123456789

DEPT/AGENCY: UNK1

CASE/REPORT: 10-00000

TEST TYPE: U

ALCO TARGET VALUE: .082

ALCO S/N: 78966

-- BREATH ANALYSIS --

.082 ADJUSTED FOR 29.70 in		
ALCO TARGET	.081	00:23
BLANK TEST	.000	00:24
INTERNAL STANDARD	VERIFIED	00:24
ALCO TV 29.70 in	.083	00:25
BLANK TEST	.000	00:25
SUBJECT SAMPLE	.000	00:26
BLANK TEST	.000	00:27
ALCO TV 29.70 in	.083	00:27
BLANK TEST	.000	00:28

AWB 12/23/10

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
 DATAMASTER cdm 130296

DECEMBER 04, 2010
 TIME 00:29

-- DIAGNOSTIC CHECK --

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 02/20/01

HEATERS

SAMPLE CHAMBER: 49c

BREATH TUBE: 41c

BAROMETER: 29.70 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!"#\$%&'()*+,-./0123456789:;<=>?@ABCDEFGHI
 HIJKLMNPOQRSTUVWXYZ[\]^_`abcdefghijklmnop
 qrstuvwxyz{|}~■