

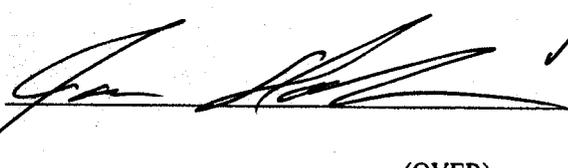
VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

SEP 23 2009

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	<u>130297</u> ✓
Name		<u>JAMES C. HOELSCHER</u>	ID# <u>5343</u> Date <u>9-21-09</u> ✓
A	Agency	<u>Hooper Bay Police Dept.</u>	Phone # <u>758-4615</u>
Instrument Location		<u>Hooper Bay Police Dept. Hooper Bay, AK</u> ✓	
Alco S/N		<u>X301526</u> ✓	Target Value <u>1.080</u> ✓ High Pressure <u>800 PSI</u>
B	Alco Test Value Average		<u>1.081</u> ✓
	1 st Alco	<u>1.080</u> ✓	2 nd Alco
Signature			
(OVER)			

BMB
10/13/09

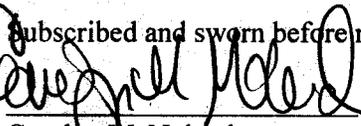
(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 20th day of October, 2009.


(Notary Seal Stamp)
Carolyn M. Noland
Notary Public, State of Alaska
Commission Expires with Office



VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130297 ✓

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

DIAGNOSTIC CHECK

Breath Test Record

Serial Number Model
 Location

Subject Information

Last Name O.L. #
 First Name

Operator Information

Operator Name Case
 Operator # Department

Test Results

Alco Target Alco Serial
 Nominal Barometer Test Type
 Dry Gas 1 Time: Test Date
 Subject Alcohol Time: Test Time
 Dry Gas 2 Time: Report

Diagnostic Test Record

Serial Number Model
 Location

Diagnostic Test Results

Test Date Computer
 Test Time Program
 Software Date
 Sample Chamber (C)
 Breath Tube (C)
 Barometer (in)
 Flow Detector
 High Speed Pump
 Detector
 Filter
 Quartz
 Calibration

ALCO 70 12:25 ✓
 BLANK TEST 000 12:22 ✓
 SUBJECT SAMPLE 000 12:24
 BLANK TEST 000 12:25
 ALCO 70 12:25 ✓
 BLANK TEST 000 12:25

BMS
10/13/09

VEHICLE: OKAY
 FILTERS: OKAY
 QUARTZ STANDARD: OKAY
 CALIBRATION: OKAY

PRINTER TEST
 10/13/09 12:25:24
 130297 130297 130297
 130297 130297 130297