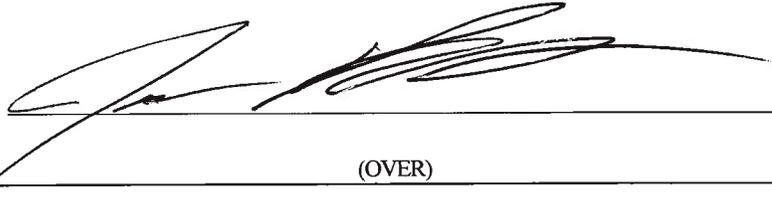


VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N <u>130297</u> ✓
Name	<u>JAMES HOELSCHER</u>	ID# <u>5343</u> Date <u>11-16-10</u> ✓
A Agency	<u>HOOPER BAY POLICE DEPT</u>	Phone # <u>758-4615</u>
Instrument Location		<u>HOOPER BAY</u>
B Alco S/N	<u>X172968</u> ✓	Target Value <u>.081</u> ✓ High Pressure <u>800 PSI</u>
Alco Test Values		<u>.079</u> ✓ 1 st Alco <u>.079</u> ✓ 2 nd Alco
Signature		

(OVER)

(Do Not write in the area below)


BMB
12/16/10


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


 Nita J. Bolz
 Scientific Director
 State Breath Alcohol Program

Subscribed and sworn before me this 23RD day of DEC, 2010.


 (Notary Seal Stamp)
 Daniel L. Nicholas
 Notary Public, State of Alaska
 Commission Expires with Office



VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N

130297 *OWJ*
12/14/10

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130297

NOVEMBER 16, 2010

OPERATOR'S NAME:
HOELSCHER/JAMES/C
OPERATOR'S NUMBER: 5343
SUBJECT'S LAST NAME:

VERIFICATION
SUBJECT'S FIRST NAME/MI :

OF CALIBRATION

O.L. #: N/A

DEPT/AGENCY: HPB1

CASE/REPORT: N/A

TEST TYPE: V

ALCO TARGET VALUE: .001

ALCO S/N: X172968

--- BREATH ANALYSIS ---

.001 ADJUSTED FOR 31.21 in
ALCO TARGET .004 13:26
BLANK TEST .000 13:26
INTERNAL STANDARD VERIFIED 13:27
ALCO TV 31.21 in .079 13:27
BLANK TEST .000 13:28
SUBJECT SAMPLE .000 13:28
BLANK TEST .000 13:29
ALCO TV 31.21 in .079 13:29
BLANK TEST .000 13:30

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130297

NOVEMBER 16, 2010
TIME 13:23

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 02/20/01
HEATERS
SAMPLE CHAMBER: 40c
BREATH TUBE: 41c
BAROMETER: 31.21 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

!"#\$%&'()*+,-./0123456789:;<=>?@ABCDEFG
HIJKLNMOPQRSTUVWXYZ[\]^_`abcde fghijklmno
pqrstuvwxyz{|}~||