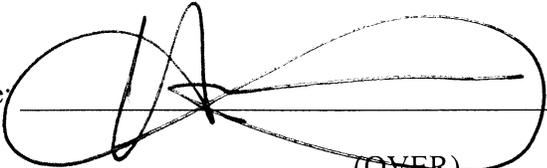


# VERIFICATION OF CALIBRATION REPORT

JUL 07 2009

Of DataMaster cdm Breath test Instrument  
State of Alaska

Scientific Crime Detection Laboratory – Statewide Breath Alcohol Program


Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N: <u>130298</u>
Name: <u>JAMES C. GIPSON</u> ID#: <u>4842</u> Date: <u>1 July 09</u>		
<b>A</b>	Agency: <u>Palmer Police Department</u> Phone #: <u>(907) 745-4811</u>	
	Instrument Location: <u>Palmer Police Department</u>	
Alco S/N: <u>X124627</u> Target Value: <u>.084</u> High Pressure: <u>500</u>		
<b>B</b>	Alco Test Value Average: <u>.084</u> <u>.085</u> 1 <sup>st</sup> Alco 2 <sup>nd</sup> Alco	
Signature:		<u>8/15/09</u>
	(OVER)	<u>BMB</u> <u>7/14/09</u>


I, Nita J. Bolz, after being first duly sworn, depose (Do not write in this area below)

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.

  
 Nita J. Bolz  
 Scientific Director  
 State Breath Alcohol Program

Subscribed and sworn before me this 20<sup>th</sup> day of July, 2009.

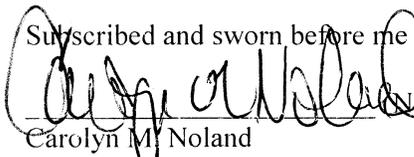  
 Carolyn M. Noland  
 Notary Public, State of Alaska  
 Commission Expires with Office



# VERIFICATION OF CALIBRATION REPORT

Of DataMaster cdm Breath test Instrument

State of Alaska

Scientific Crime Detection Laboratory – Statewide Breath Alcohol Program

DataMaster cdm S/N: 130298 ✓

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130298

JULY 01, 2009

OPERATOR'S NAME: GIPSON/JANES/C  
OPERATOR'S NUMBER: 4842  
SUBJECT'S LAST NAME: VERIFICATION OF CAL  
SUBJECT'S FIRST NAME/MI: RUDSO  
O.L. #: 0123456  
DEPT/AGENCY: PLM1  
ORGE/REPORT: 01-1234  
TEST TYPE: U  
ALCO TARGET VALUE: .084 ✓  
ALCO S/N: X124627

### --- BREATH ANALYSIS ---

.084 ADJUSTED FOR 30.37 in  
ALCO TARGET .085 08:19  
BLANK TEST .000 08:20  
INTERNAL STANDARD (VERIFIED) 08:20  
ALCO TV 30.37 in .084 ✓ 08:21  
BLANK TEST .000 08:21  
SUBJECT SAMPLE .000 08:22  
BLANK TEST .000 08:23 ✓  
ALCO TV 30.37 in .085 08:23  
BLANK TEST .000 08:24

*Bmg*  
*7/14/09*

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130298

JULY 01, 2009 ✓  
TIME 08:17

### --- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 02/20/01  
HEATERS  
SAMPLE CHAMBER: 49c  
BREATH TUBE: 41c  
BAROMETER: 30.35 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

### PRINTER TEST

!##%&'()\*+,-./0123456789:;<=>?@ABCDEFGHI  
HIJKLMNPOQRSTUVWXYZ[\]^\_`abcde fghijklmno  
pqrstuvwxyz{|}~