

VERIFICATION OF CALIBRATION REPORT

Of DataMaster cdm Breath test Instrument

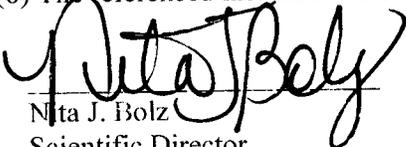
State of Alaska

Scientific Crime Detection Laboratory – Statewide Breath Alcohol Program

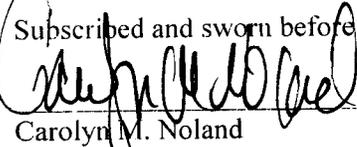
AUG 14 2009

DataMaster cdm S/N: <u>130298</u> ✓	
Supervisor/Operator Performing the Verification Procedure:	
Name: <u>JAMES C. GIPSON</u> ID#: <u>4842</u> Date: <u>30 July 09</u> ✓	
A	Agency: <u>Palmer Police Department</u> Phone #: <u>(907) 745-4811</u>
Instrument Location: <u>Palmer Police Department</u>	
Alco S/N: <u>77199</u> Target Value: <u>.076</u> High Pressure: <u>700</u>	
B	Alco Test Value Average: <u>.075</u> <u>.074</u>
	1 st Alco 2 nd Alco
Signature:  ✓	
(OVER)	
<u>CS</u> <u>8/27/09</u>	

- (Do Not write in the area below)
- I, Nita J. Bolz, after being first duly sworn, depose and state as follows:
- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
 - (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
 - (3) I am the Scientific Director of the State Breath Alcohol Program.
 - (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
 - (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
 - (6) The referenced instrument is certified for evidentiary use in the State of Alaska


Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 16th day of Sept., 2009.

 (Notary Seal Stamp)
Carolyn M. Noland
Notary Public, State of Alaska
Commission Expires with Office



VERIFICATION OF CALIBRATION REPORT

Of DataMaster cdm Breath test Instrument

State of Alaska

Scientific Crime Detection Laboratory – Statewide Breath Alcohol Program

DataMaster cdm S/N: 130298

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES

NONDRINKING SUBJECT TEST

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130298

JULY 30, 2009

OPERATOR'S NAME: *CS 8/27/09*
GIPSON, JAMES/C
OPERATOR'S NUMBER: 4042
SUBJECT'S LAST NAME:
VERIFICATION OF CAL
SUBJECT'S FIRST NAME/MI :
RUCSW

O.L. #: 0123456
DEPT/AGENCY: PLM1
CASE/REPORT: 01-2345
TEST TYPE: U
ALCO TARGET VALUE: .076
ALCO S/N: 77199

— BREATH ANALYSIS —

.076 ADJUSTED FOR 29.91 in
ALCO TARGET .075 14:24
BLANK TEST .000 14:25
INTERNAL STANDARD VERIFIED 14:25
ALCO TU 29.91 in .075 14:25
BLANK TEST .000 14:26
SUBJECT SAMPLE *CS 8/27/09* .000 14:27
BLANK TEST .000 14:27
ALCO TU 29.91 in .074 14:28
BLANK TEST .000 14:28

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130298

JULY 30, 2009
TIME 14:15

— DIAGNOSTIC CHECK —

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 02/20/01
HEATERS
SAMPLE CHAMBER: 48c
BREATH TUBE: 43c
BAROMETER: 29.91 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

! " # \$ % & ' () * + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G
H I J K L M N O P Q R S T U V W X Y Z [\] ^ _ ` a b c d e f g h i j k l m n o
p q r s t u v w x y z () * + , - . /