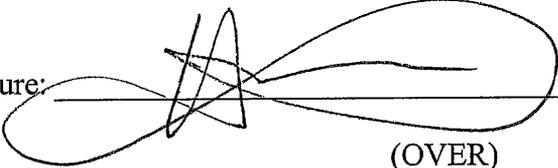


VERIFICATION OF CALIBRATION REPORT

Of DataMaster cdm Breath test Instrument

State of Alaska

Scientific Crime Detection Laboratory – Statewide Breath Alcohol Program DEC 10 2008

DataMaster cdm S/N: <u>130298</u> ✓		
Supervisor/Operator Performing the Verification Procedure:		
Name: <u>JAMES C. GIPSON</u> ID#: <u>4842</u> Date: <u>2 December 09</u> ¹⁰ 2008		
A	Agency: <u>Palmer Police Department</u> Phone #: <u>(907) 745-4811</u>	
	Instrument Location: <u>Palmer Police Department</u> ✓	
Alco S/N: <u>78268</u> ✓ Target Value: <u>.077</u> ✓ High Pressure: <u>1300</u>		
B	Alco Test Value Average: <u>.080</u> ✓ <u>.080</u> ✓ 1 st Alco 2 nd Alco	
Signature:  ✓		<u>CSB</u> <u>12/18/08</u>
(OVER)		

Under the Alaska Rules of Evidence, I certify that:
(Do Not write in the area below)


(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Jim Gipson, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed,





Jeanne Swartz
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

12/20/08

Date

VERIFICATION OF CALIBRATION REPORT

Of DataMaster cdm Breath test Instrument

State of Alaska

Scientific Crime Detection Laboratory – Statewide Breath Alcohol Program

DataMaster cdm S/N: 130298 ✓

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130298

DECEMBER 02, 2008

OPERATOR'S NAME:
GIPSON, JAMES/C
OPERATOR'S NUMBER: 4842
SUBJECT'S LAST NAME:
VERIFICATION OF CAL
SUBJECT'S FIRST NAME/MI :
RJC50

O.L. #: 0123456
DEPT/AGENCY: PLM1
CASE/REPORT: 01-2345
TEST TYPE: V
ALCO TARGET VALUE: .077 ✓
ALCO S/N: 70268

— BREATH ANALYSIS —

.077 ADJUSTED FOR 30.38 in
ALCO TARGET .078 16:23
BLANK TEST .000 16:24
INTERNAL STANDARD VERIFIED 16:24
ALCO TV 30.38 in .000 ✓ 16:24
BLANK TEST .000 16:25
SUBJECT SAMPLE .000 16:26
BLANK TEST .000 16:26
ALCO TV 30.40 in .000 ✓ 16:27
BLANK TEST .000 16:27

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130298

DECEMBER 02, 2008 ✓
TIME 16:17

— DIAGNOSTIC CHECK —

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 02/20/01
HEATERS
SAMPLE CHAMBER: 49c
BREATH TUBE: 42c
BAROMETER: 30.38 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

! " # % & ' () * + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G
H I J K L M N O P Q R S T U V W X Y Z I \] ^ _ ` a b c d e f g h i j k l m n o
p q r s t u v w x y z { } ~ ¡ ¢