

OCT 26 2009

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument
State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

OCT 26 2009

Supervisor/Operator Performing the Verification Procedure: DataMaster cdm S/N 130299 ✓

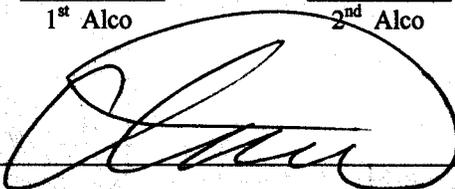
Name Chris Babcock ID# 3867 Date 10-20-09 ✓

A Agency King Cove PD Phone # 497-2210

Instrument Location King Cove Police Department 11-9-09
CWW ✓

B Alco S/N X301600 ✓ Target Value .080 ✓ High Pressure 1000 PSI

Alco Test Values .078 ✓ .078 ✓
1st Alco 2nd Alco

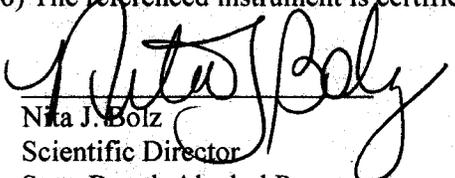
Signature 

(OVER)

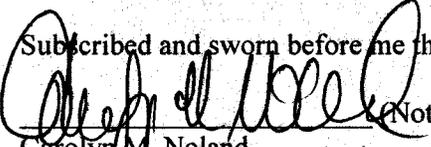
PMB
11/14/09

(Do Not write in the area below)

- I, Nita J. Bolz, after being first duly sworn, depose and state as follows:
- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
 - (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
 - (3) I am the Scientific Director of the State Breath Alcohol Program.
 - (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
 - (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
 - (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


 Nita J. Bolz
 Scientific Director
 State Breath Alcohol Program

Subscribed and sworn before me this 3rd day of Dec, 2009.


 Carolyn M. Noland
 Notary Public, State of Alaska
 Commission Expires with Office



VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130299

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

[Empty box for taping test strip]

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130299

OCTOBER 20, 2009

OPERATOR'S NAME:
BRADCOCK CHRIS M
OPERATOR'S NUMBER: 3067
SUBJECT'S LAST NAME:
UOC

SUBJECT'S FIRST NAME/MI:
UOC

O.L. #: 123456
DEPT/AGENCY: KUC1
CASE/REPORT: UOC
TEST TYPE: U
ALCO TARGET VALUE: .000
ALCO S/N: X301600

--- BREATH ANALYSIS ---

.000 ADJUSTED FOR 29.67 in

ALCO TARGET	.000	12:56
BLANK TEST	.000	12:57
INTERNAL STANDARD	VERIFIED	12:57
ALCO TV 29.67 in	.078	12:57
BLANK TEST	.000	12:58
SUBJECT SAMPLE	.000	12:59
BLANK TEST	.000	13:00
ALCO TV 29.67 in	.078	13:00
BLANK TEST	.000	13:01

DIAGNOSTIC CHECK

[Empty box for taping test strip]

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130299

OCTOBER 20, 2009
TIME 12:53

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 02/20/01
HEATERS
SAMPLE CHAMBER: 48c
BREATH TUBE: 42c
BAROMETER: 29.67 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

ALCO TV 29.67 in .078
BT 06/03