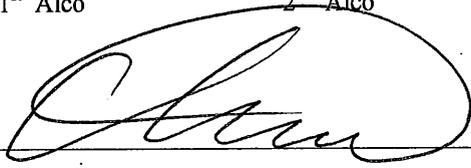


# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130299 ✓
Name		Christopher M Babcock	ID# 3867 Date 11-3-08 ✓
A	Agency	King Cove PD	Phone # 497-2210
Instrument Location		Squad room ✓	
Alco S/N		X172971 ✓	Target Value .078 ✓ High Pressure 1000 ✓
Alco Test Values		.081 ✓	.081 ✓
		1 <sup>st</sup> Alco	2 <sup>nd</sup> Alco
Signature		 CSB 11/8/08	
(OVER)			

Under the Alaska Rules of Evidence, I certify that, (Do Not write in the area below)

(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Christopher M Babcock, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed,





Jeanne Swartz  
Scientific Director Designee  
State of Alaska  
State Breath Alcohol Testing Program

11/19/08  
Date

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130299 ✓

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130299

NOVEMBER 03, 2008

OPERATOR'S NAME:  
BABCOCK CHRISTOPHER M

OPERATOR'S NUMBER: 3867

SUBJECT'S LAST NAME:

UOC

SUBJECT'S FIRST NAME/NI:

UOC

Q.L. #: 123456

DEPT/AGENCY: KUC1

CASE/REPORT: UOC

TEST TYPE: U

ALCO TARGET VALUE: .078 ✓

ALCO S/N: K172971

--- BREATH ANALYSIS ---

.078 ADJUSTED FOR 30.16 in

ALCO TARGET	.078	08:49
BLANK TEST	.000	08:50
INTERNAL STANDARD	VERIFIED	08:50
ALCO TV 30.16 in	.081 ✓	08:50
BLANK TEST	.000	08:51
SUBJECT SAMPLE	.000	08:51
BLANK TEST	.000	08:52
ALCO TV 30.16 in	.081 ✓	08:53
BLANK TEST	.000	08:53

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130299

NOVEMBER 03, 2008 ✓

TIME 08:47

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 02/20/01

HEATERS

SAMPLE CHAMBER: 48c

BREATH TUBE: 41c

BAROMETER: 30.16 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!"#\$%&'()\*+,-./0123456789:;<=>?@ABCDEFGHIJ  
KLMNOPQRSTUVWXYZ[\]^\_`abcdefghijklmnop  
qrstuvwxy{|}~■