

VERIFICATION OF CALIBRATION REPORT

DataMaster cdm breath Test Instrument
State of Alaska

APR 16 2010

Scientific Crime Detection Laboratory - statewide Breath Alcohol Program

A

DataMaster cdm S/N 130299 ✓

Supervisor/Operator Performing the Verification Procedure:

Name: Chris Babcock

ID#: 3867

Date: 4/12/2010 ✓

Agency: King Cove Department of Public Safety

Phone #: 497-2210

Instrument Location: Squad Room

B

Alco S/N: X124634 ✓

Target Value: .078 ✓

High Pressure: 900psi

Alco Test Value Average:

.077 ✓

1st Alco

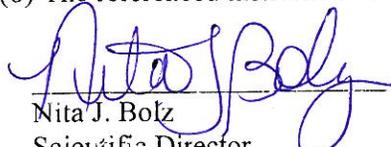
.077 ✓

2nd Alco

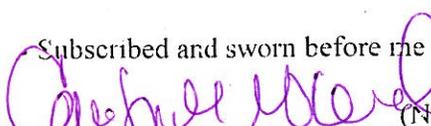
(OVER)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


 Nita J. Bolz
 Scientific Director
 State Breath Alcohol Program

Subscribed and sworn before me this 20th day of April, 2010.


 (Notary Seal Stamp)

Carolyn M. Noland
 Notary Public, State of Alaska
 Commission Expires with Office



COB
4/26/10

VERIFICATION OF CALIBRATION REPORT

Of DataMaster cdm breath Test Instrumen

State of Alaska

Scientific Crime Detection Laboratory – statewide Breath Alcohol Program

C

DataMaster cdm S/N 130299

(CONTINUED FROM FRONT PAGE)

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130299 ✓

APRIL 12, 2010 ✓ *COS 4/26/10*

OPERATOR'S NAME:
BABCOCK CHRISTOPHER M
OPERATOR'S NUMBER: 3867
SUBJECT'S LAST NAME:
UOC
SUBJECT'S FIRST NAME/MI :
UOC
O.L. #: 123456
DEPT/AGENCY: KUC1
CASE/REPORT: UOC
TEST TYPE: U ✓
ALCO TARGET VALUE: .078 ✓
ALCO S/N: X124634 ✓

--- BREATH ANALYSIS --- ✓

.078 ADJUSTED FOR 30.03 in		
ALCO TARGET	.078	12:59
BLANK TEST	.000	13:00
INTERNAL STANDARD	VERIFIED	13:00
ALCO TO 30.04 in	.077 ✓	13:00
BLANK TEST	.000	13:01
SUBJECT SAMPLE	.000	13:01
BLANK TEST	.000	13:02
ALCO TO 30.03 in	.077 ✓	13:03
BLANK TEST	.000	13:03

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130299 ✓

APRIL 12, 2010 ✓
TIME 12:56 ✓

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 02/20/01

HEATERS
SAMPLE CHAMBER: 42c
BREATH TUBE: 41c

BAROMETER: 30.03 in

FLOW DETECTOR: OKAY

PUMP
HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST
!"#\$%&'()*+,-./0123456789:;<=>?@ABCDEFGHIJKL
MNOPQRSTUVWXYZ[\]^_`ab cde fgh i jklmno
pqrstu vwxyz{|}~#