

VERIFICATION OF CALIBRATION REPORT
Of DataMaster cdm breath Test Instrument
State of Alaska
Scientific Crime Detection Laboratory – statewide Breath Alcohol Program

JUN 22 2010

A **DataMaster cdm S/N 130299** ✓

Supervisor/Operator Performing the Verification Procedure:

Name: Chris Babcock ID#: 3867 ✓ Date: 6/12/2010 *6/14/10 ocd*
6/23/10

Agency: King Cove Department of Public Safety Phone #: 497-2210

Instrument Location: Squad Room

B

Alco S/N: X124634 ✓ Target Value: .078 ✓ High Pressure: 900psi

Alco Test Value Average: .078 ✓ .078 ✓
1st Alco 2nd Alco


(OVER)



I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


AMB
6/23/10

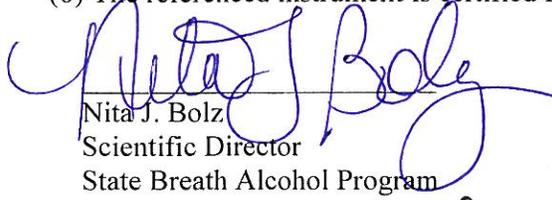


Nita J. Bolz
Scientific Director
State Breath Alcohol Program



Subscribed and sworn before me this 21st day of July, 2010.

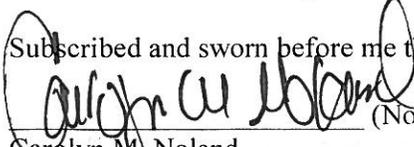

(Notary Seal Stamp)
Carolyn M. Noland
Notary Public, State of Alaska
Commission Expires with Office

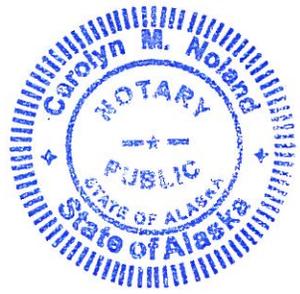

VERIFICATION OF CALIBRATION REPORT
Of DataMaster cdm breath Test Instrument
State of Alaska
Scientific Crime Detection Laboratory – statewide Breath Alcohol Program

C **DataMaster cdm S/N 130299**

(CONTINUED FROM FRONT PAGE)

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
 DATAMASTER cdm 130299

JUNE 11, 2010

OPERATOR'S NAME: *BMB 6/23/10*
 BABCOCK CHRISTOPHER M
 OPERATOR'S NUMBER: 3867
 SUBJECT'S LAST NAME:
 UOC
 SUBJECT'S FIRST NAME/MI :
 UOC
 O.L. #: 123456
 DEPT/AGENCY: KUC1
 CASE/REPORT: UOC
 TEST TYPE: U
 ALCO TARGET VALUE: .078
 ALCO S/N: X124634

--- BREATH ANALYSIS ---

.078 ADJUSTED FOR 30.14 in		
ALCO TARGET	.078	11:06
BLANK TEST	.000	11:07
INTERNAL STANDARD	VERIFIED	11:07
ALCO TV 30.14 in	.078	11:08
BLANK TEST	.000	11:08
SUBJECT SAMPLE	.000	11:09
BLANK TEST	.000	11:09
ALCO TV 30.14 in	.078	11:10
BLANK TEST	.000	11:11

BMB 6/23/10

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
 DATAMASTER cdm 130299

JUNE 11, 2010
 TIME 11:04

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY
 PROGRAM: OKAY
 SOFTWARE DATE: 02/20/01

HEATERS
 SAMPLE CHAMBER: 49c
 BREATH TUBE: 41c

BAROMETER: 30.14 in

FLOW DETECTOR: OKAY

PUMP
 HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!"#\$%&'()*+,-./0123456789:;<=>?@ABCDEFGHIJKL
 MNOPQRSTUVWXYZ[\]^_`abcdefgijklmnop
 qrstuvwxyz{|}~@