

**VERIFICATION OF CALIBRATION REPORT**  
*of DataMaster cdm Breath Test Instrument*  
 State of Alaska  
 Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

OCT 27 2010

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N <u>130299</u> ✓
Name <u>Christopher M Babcock</u>	ID# <u>3867</u> ✓	Date <u>10/25/2010</u> ✓
A Agency <u>King Cove Dept. of Public Safety</u>		Phone # <u>497-2210</u>
Instrument Location <u>Squad Room</u>		
B Alco S/N <u>X124634</u> ✓		Target Value <u>.078</u> ✓
		High Pressure <u>400</u>
Alco Test Values	<u>.077</u> ✓ 1 <sup>st</sup> Alco	<u>.077</u> ✓ 2 <sup>nd</sup> Alco
Signature 		
(OVER)		

*CMB*  
12/9/10


(Do Not write in the area below)


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

  
 Nita J. Bolz  
 Scientific Director  
 State Breath Alcohol Program

Subscribed and sworn before me this 22<sup>nd</sup> day of DEC, 2010.

 (Notary Seal Stamp)  
 Daniel L. Nicholas  
 Notary Public, State of Alaska  
 Commission Expires with Office

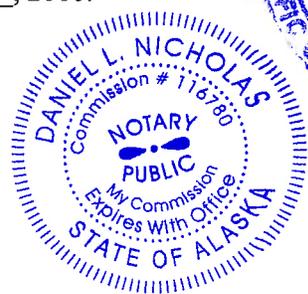

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130299

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130299

OCTOBER 25, 2010

OPERATOR'S NAME:

BOESCHK CHRISTOPHER M

OPERATOR'S NUMBER: 3867

SUBJECT'S LAST NAME:

UOC

SUBJECT'S FIRST NAME/MI :

UOC

D.L. #: 123456

DEPT/AGENCY: KUC1

CRSE/REPORT: UOC

TEST TYPE: U

ALCO TARGET VALUE: .078

ALCO S/N: X124634

--- BREATH ANALYSIS ---

.078 ADJUSTED FOR 29.78 in  
ALCO TARGET .077 13:03  
BLANK TEST .000 13:04  
INTERNAL STANDARD VERIFIED 13:04  
ALCO TV 29.78 in .077 13:04  
BLANK TEST .000 13:05  
SUBJECT SAMPLE .000 13:06  
BLANK TEST .000 13:06  
ALCO TV 29.78 in .077 13:07  
BLANK TEST .000 13:07

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130299

OCTOBER 25, 2010

TIME 12:58

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 02/20/01

HEATERS  
SAMPLE CHAMBER: 49c  
BREATH TUBE: 42c

BAROMETER: 29.78 in

FLOW DETECTOR: OKAY

PUMP  
HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!@#%&'()\*+,-./0123456789:;<=>?@BCDEFG  
HIJKL NOPQRSTU VWXYZ[\]^\_`'abcde fghijklmno  
pqrstuvwxy z{|}~■