

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument


State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N <u>130299</u>	
Name	<u>Christopher M Babcock</u>	ID#	<u>3867</u> Date <u>12/14/10</u>
A Agency	<u>King Cove Dept. of Public Safety</u>		Phone # <u>497-2210</u>
Instrument Location	<u>Squad Room</u>		
B Alco S/N	<u>X124634</u>	Target Value	<u>.078</u> High Pressure <u>400</u>
Alco Test Values	<u>.078</u>	<u>.078</u>	
	1 <sup>st</sup> Alco	2 <sup>nd</sup> Alco	
Signature			<u>CB</u> <u>12/30/10</u>
(OVER)			

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:


- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska. 130299 12/14/10

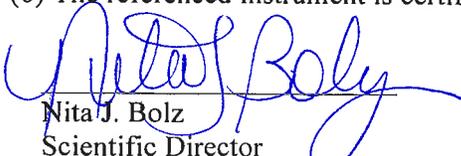  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 18<sup>th</sup> day of JAN, 2011 DM

 (Notary Seal Stamp)

Daniel L. Nicholas  
Notary Public, State of Alaska  
Commission Expires with Office



NJB  
1/18/11

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130299

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130299

DECEMBER 14, 2010

OPERATOR'S NAME:  
BARROCK CHRISTOPHER M  
OPERATOR'S NUMBER: 3867  
SUBJECT'S LAST NAME:  
UOC  
SUBJECT'S FIRST NAME/MI :  
UOC

D.L. #: 123456  
DEPT/AGENCY: KVC1  
CASE/REPORT: UOC  
TEST TYPE: U  
ALCO TARGET VALUE: .078  
ALCO S/N: K124634

--- BREATH ANALYSIS ---

.078 ADJUSTED FOR 30.14 in  
ALCO TARGET .078 13:00  
BLANK TEST .000 13:01  
INTERNAL STANDARD VERIFIED 13:01  
ALCO TO 30.14 in .078 13:01  
BLANK TEST .000 13:02  
SUBJECT SAMPLE .000 13:03  
BLANK TEST .000 13:04  
ALCO TO 30.14 in .078 13:04  
BLANK TEST .000 13:05

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130299

DECEMBER 14, 2010  
TIME 12:57

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 02/20/01  
HEATERS  
SAMPLE CHAMBER: 48c  
BREATH TUBE: 42c  
BAROMETER: 30.14 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

PRINTER TEST

!"#\$%&'()\*+,-./0123456789:;<=>?@ABCDEF6  
HIJKL NOPQRSTU VWXYZ[\]^\_`'abcde fghijklmno  
pqrstu vwxyz{|}~