

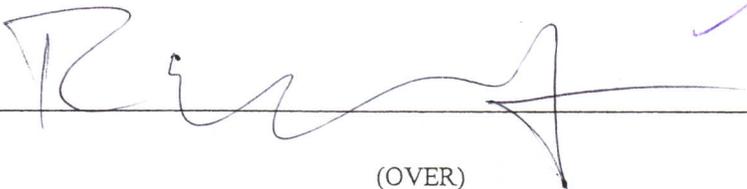
# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

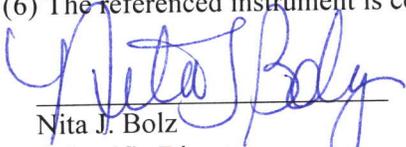
MAR 23 2010

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N <u>130301</u> <del>X301583</del> (P93-19-10)	
Name <u>CLAY FARIS</u>		ID# <u>6170</u>	Date <u>3-14-10</u>
A	Agency <u>FBK7</u>	Phone # <u>(907) 474-7721</u>	
Instrument Location <u>UAF Police Dept</u>			
Alco S/N <u>X301583</u>		Target Value <u>.084</u>	High Pressure <u>550 psi.</u>
B	Alco Test Value Average <u>.085</u>	<u>.085</u>	
	1 <sup>st</sup> Alco	2 <sup>nd</sup> Alco	
Signature 			
(OVER)			

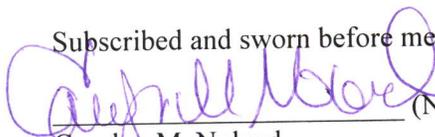
BMB  
3/24/10

I, Nita J. Bolz, after being first duly sworn, depose and state as follows (in the area below)


- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 15<sup>th</sup> day of April, 2010.

  
(Notary Seal Stamp)

Carolyn M. Noland  
Notary-Public, State of Alaska  
Commission Expires with Office



# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument  
State of Alaska  
Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130301 ✓

(CONTINUED FROM FRONT PAGE)

**C** TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130301

MARCH 14, 2010 ✓

OPERATOR'S NAME: **OMB 3/24/10**  
FARIS/CLAY  
OPERATOR'S NUMBER: 6170  
SUBJECT'S LAST NAME:  
VERIFICATION OF CAL  
SUBJECT'S FIRST NAME/MI :  
VOC

O.L. #: VOC  
DEPT/AGENCY: FBK7  
CASE/REPORT:  
TEST TYPE: U  
ALCO TARGET VALUE: .084 ✓  
ALCO S/N: X301583

--- BREATH ANALYSIS ---

.084 ADJUSTED FOR 29.16 in		
ALCO TARGET	.081	06:25
BLANK TEST	.000	06:26
INTERNAL STANDARD	VERIFIED	06:26
ALCO TV 29.16 in	.085	06:27
BLANK TEST	.000	06:28
SUBJECT SAMPLE	.000	06:28
BLANK TEST	.000	06:29
ALCO TV 29.16 in	.085	06:30
BLANK TEST	.000	06:30

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130301

MARCH 14, 2010 ✓  
TIME 06:22

--- DIAGNOSTIC CHECK ---

COMPUTER:	OKAY
PROGRAM:	OKAY
SOFTWARE DATE:	02/20/01
HEATERS	
SAMPLE CHAMBER:	49c
BREATH TUBE:	42c
BAROMETER:	29.16 in
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

PRINTER TEST

!"#\$%&'()\*+,-./0123456789:;<=>?@ABCDEFGHI  
HIJKLMNPOQRSTUVWXYZ[\]^\_`abcde fghi jklmno  
pqrstuvwxyz{|}~■