

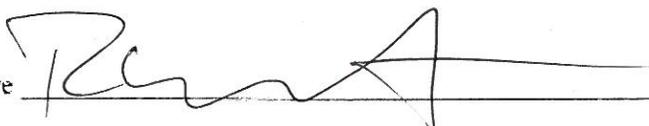
VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

JUL 21 2010

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N <u>130301</u> ✓
Name	<u>CLAY FARIS</u>	ID# <u>6170</u> ✓ Date <u>7-17-10</u> ✓ <small>17 (RF) ✓</small>
A Agency	<u>UNIVERSITY POLICE DEPT. - FBKS</u>	Phone # <u>(907) 474-7721</u>
Instrument Location <u>UNIVERSITY POLICE DEPT. - FBKS</u>		
B Alco S/N <u>X172931</u> ✓ Target Value <u>.082</u> ✓ High Pressure <u>1350 psi</u>		
Alco Test Values		
	<u>.086</u> ✓ 1 st Alco	<u>.085</u> ✓ 2 nd Alco
Signature		<u>003</u> <u>7/23/10</u>
(OVER)		

(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 9th day of AUGUST, 2010.

 (Notary Seal Stamp)
Daniel L. Nicholas
Notary Public, State of Alaska
Commission Expires with Office



VERIFICATION OF CALIBRATION REPORT
of DataMaster cdm breath Test Instrument
State of Alaska
Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130301

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
 DATAMASTER cdm 130301

JULY 17, 2010

CAS #130310

OPERATOR'S NAME:
 FARIS/CLAY
 OPERATOR'S NUMBER: 6170
 SUBJECT'S LAST NAME:
 VERIFICATION OF CAL
 SUBJECT'S FIRST NAME/MI :
 VUC
 O.L. #: VUC
 DEPT/AGENCY: FBK7
 CASE/REPORT: VUC
 TEST TYPE: U
 ALCO TARGET VALUE: .082
 ALCO S/N: X172931

--- BREATH ANALYSIS ---

.082 ADJUSTED FOR 29.72 in
 ALCO TARGET .081 00:20
 BLANK TEST .000 00:20
 INTERNAL STANDARD VERIFIED 00:21
 ALCO TV 29.72 in .086 00:21
 BLANK TEST .000 00:22
 SUBJECT SAMPLE *CAS #130310* .080 00:23
 BLANK TEST .000 00:23
 ALCO TV 29.70 in .085 00:24
 BLANK TEST .000 00:25

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
 DATAMASTER cdm 130301

JULY 17, 2010
 TIME 00:17

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY
 PROGRAM: OKAY
 SOFTWARE DATE: 02/20/01
 HEATERS
 SAMPLE CHAMBER: 49c
 BREATH TUBE: 42c
 BAROMETER: 29.72 in
 FLOW DETECTOR: OKAY
 PUMP
 HIGH SPEED: OKAY
 DETECTOR: OKAY
 FILTERS: OKAY
 QUARTZ STANDARD: OKAY
 CALIBRATION: OKAY

PRINTER TEST

!"#\$%&'()*+,-./0123456789:;<=>?@ABCDEFG
 HIJKLMNOPQRSTUVWXYZ[\]^_`abcdefgijklmnop
 qrstuvwxyz{|}~