


VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

| | | |
|--|--|---|
| Supervisor/Operator Performing the Verification Procedure: | | DataMaster cdm S/N <u>130302</u> ✓ |
| Name | <u>Officer Kevin Nelson</u> | ID# <u>5349</u> ✓ Date <u>6/17/08</u> |
| A Agency | <u>North Pole Police Department</u> ✓ | Phone # <u>(907)488-0612</u> |
| Instrument Location | <u>125 Snowman Lane, North Pole, AK 99705</u> | |
| B Alco S/N | <u>X124634</u> ✓ | Target Value <u>.081</u> ✓ High Pressure <u>300 psi</u> |
| Alco Test Values | <u>.081</u> ✓ 1 st Alco | <u>.081</u> ✓ 2 nd Alco |
| Signature |  | <u>CSB</u> <u>6/27/08</u> |

(OVER)

(Do Not write in the area below)


Under the Alaska Rules of Evidence, I certify that;


(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Kevin Nelson, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed,

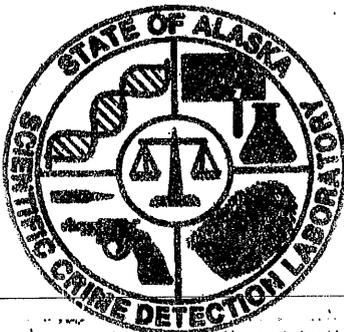



Jeanne Swartz
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

6/30/08
Date

BT9 06/03
JUN 19 2008

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130302 ✓

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130302

JUNE 17, 2008 ✓ *CS 6/21/08*

OPERATOR'S NAME:
NELSON, KEVIN HOON
OPERATOR'S NUMBER: 5349
SUBJECT'S LAST NAME:
VOC

SUBJECT'S FIRST NAME/MI:
VOC

O.L. #: 0000000
DEPT/AGENCY: NPLI
CASE/REPORT: 08-00000
TEST TYPE: V
ALCO TARGET VALUE: .081 ✓
ALCO S/N: X124634 ✓

--- BREATH ANALYSIS ---

.081 ADJUSTED FOR 29.73 in
ALCO TARGET .080 08:08
BLANK TEST .000 08:09
INTERNAL STANDARD VERIFIED 08:09
ALCO TV 29.73 in .081 ✓ 08:10
BLANK TEST .000 08:11
SUBJECT SAMPLE .000 *CS 6/21/08* 08:11
BLANK TEST .000 *CS 6/21/08* 08:12
ALCO TV 29.73 in .081 ✓ 08:13
BLANK TEST .000 08:14

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130302

JUNE 17, 2008 ✓
TIME 08:06

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 02/20/01
HEATERS
SAMPLE CHAMBER: 49c
BREATH TUBE: 41c
BAROMETER: 29.73 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

! " # % & ' () * + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G
H I J K L M N O P Q R S T U V W X Y Z [\] ^ _ ` a b c d e f g h i j k l m n o
p q r s t u v w x y z { | } ~