

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

JAN 19 2010

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	<u>130302</u>
Name	<u>Brian Mitchell</u>	ID#	<u>4119</u> Date <u>1-9-10</u>
A Agency	<u>Alaska State Troopers</u>	Phone #	<u>486-4121</u>
Instrument Location <u>Kodrak Post, Interview Room</u>			
Alco S/N <u>X124626</u>		Target Value	<u>.082</u> High Pressure <u>400</u>
Alco Test Value Average <u>.087</u>		<u>.087</u>	
1 st Alco		2 nd Alco	
Signature <u>Brian Mitchell</u>		<u>CB</u> <u>1/29/10</u>	

(OVER)

(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:


- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

Nita J. Bolz
Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 26th day of January, 2010.

Carolyn M. Noland (Notary Seal Stamp)

Carolyn M. Noland
Notary Public, State of Alaska
Commission Expires with Office

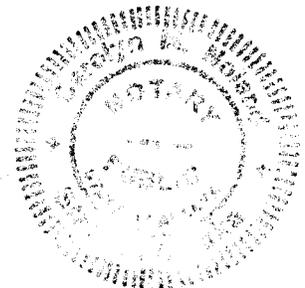

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130302

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130302

JANUARY 09, 2010

OPERATOR'S NAME: *CBS*
MITCHELL BRIAN S
OPERATOR'S NUMBER: 4119
SUBJECT'S LAST NAME: *1/22/10*
VOC
SUBJECT'S FIRST NAME/MI :
VOC
O.L. #: VOC
DEPT/AGENCY: K030
CASE/REPORT: X X X
TEST TYPE: V
ALCO TARGET VALUE: .082
ALCO S/N: X124626

--- BREATH ANALYSIS ---

.082 ADJUSTED FOR 29.41 in
ALCO (ARGE) .080 22:14
BLANK TEST .000 22:16
INTERNAL STANDARD .000 22:16
ALCO TV 29.42 in .087 22:16
BLANK TEST .000 22:17
SUBJECT SAMPLE *CBS* .080 22:18
BLANK TEST *1/22/10* .000 22:18
ALCO TV 29.41 in .087 22:19
BLANK TEST .000 22:19

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130302

JANUARY 09, 2010
TIME 22:21

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 01/06/09
HEATERS
SAMPLE CHAMBER: 43c
BREATH TUBE: 42c
BAROMETER: 29.41 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

! " # % & ' () * + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G
H I J K L M N O P Q R S T U V W X Y Z [\] ^ _ ` a b c d e f g h i j k l m n o
p q r s t u v w x y z { | } ~