

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N <u>130 303</u> ✓	
Name	<u>DARYL RICE</u>	ID#	<u>2088</u> Date <u>03/01/08</u>
A Agency	<u>SITKA POLICE DEPT.</u>	Phone #	<u>747-3245</u>
Instrument Location <u>304 LAKE STREET</u>			
Alco S/N <u>X301765</u> ✓		Target Value	<u>.083</u> ✓ High Pressure <u>800</u>
B Alco Test Values		<u>.083</u> ✓	<u>.082</u>
		1 <sup>st</sup> Alco	2 <sup>nd</sup> Alco
Signature <u>Daryl Rice</u>		<u>CS</u> <u>3/6/08</u>	

(OVER)


(Do Not write in the area below)

Under the Alaska Rules of Evidence, I certify that;

(a) I am Jeanne Swartz, Criminalist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Daryl Rice, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

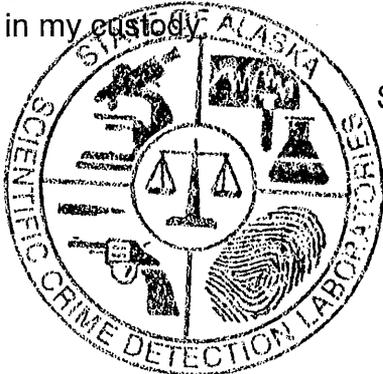

Signed and sealed,

Jeanne Swartz

Jeanne Swartz  
Scientific Director Designee  
State of Alaska  
State Breath Alcohol Testing Program

3/6/08  
Date

**VERIFICATION OF CALIBRATION REPORT**  
*of DataMaster cdm breath Test Instrument*  
*State of Alaska*  
*Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program*

DataMaster cdm S/N 130303

(CONTINUED FROM FRONT PAGE)

**C** TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

**NONDRINKING SUBJECT TEST**

ALASKA DEPARTMENT OF PUBLIC SAFETY  
 DATAMASTER cdm 130303  
 MARCH 01, 2008  
 OPERATOR'S NAME: RICE DARVYL DEAN  
 OPERATOR'S NUMBER: 2068  
 SUBJECT'S LAST NAME:  
 VERIFICATION OF CAL  
 SUBJECT'S FIRST NAME/MI :  
 UOC  
 O.L. #: VOC  
 DEPT/AGENCY: SIT1  
 CASE/REPORT: VOC  
 TEST TYPE: V  
 ALCO TARGET VALUE: .083  
 ALCO S/N: X301765 ✓

--- BREATH ANALYSIS ---

.083 ADJUSTED FOR 30.22 in		
ALCO TARGET	.083	21:35
BLANK TEST	.000	21:36
INTERNAL STANDARD	VERIFIED	21:36
ALCO TV 30.22 in	.083	21:36
BLANK TEST	.000	21:37
SUBJECT SAMPLE	.000	21:38
BLANK TEST	.000	21:38
ALCO TV 30.22 in	.082	21:39
BLANK TEST	.000	21:40

**DIAGNOSTIC CHECK**

ALASKA DEPARTMENT OF PUBLIC SAFETY  
 DATAMASTER cdm 130303  
 MARCH 01, 2008  
 TIME 21:40  
 --- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
 PROGRAM: OKAY  
 SOFTWARE DATE: 02/20/01  
 HEATERS  
 SAMPLE CHAMBER: 49c  
 BREATH TUBE: 43c  
 BAROMETER: 30.22 in  
 FLOW DETECTOR: OKAY  
 PUMP  
 HIGH SPEED: OKAY  
 DETECTOR: OKAY  
 FILTERS: OKAY  
 QUARTZ STANDARD: OKAY  
 CALIBRATION: OKAY

PRINTER TEST

```
!""#%&'()*+,-./0123456789:;{=}~?@ABCDEFGHIJ
KLMNOPQRSTUVWXYZ[\]^_`abcde fghijklmno
pqrstuvwxy{|}~■
```