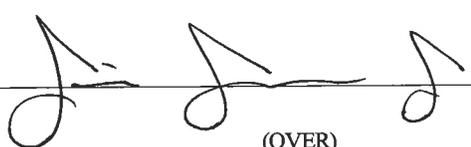


# VERIFICATION OF CALIBRATION REPORT

*of DataMaster cdm Breath Test Instrument  
State of Alaska*

*Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program*


DataMaster cdm S/N <u>134343</u> ✓	
Supervisor/Operator Performing the Verification Procedure:	
Name <u>JAMES I. JENSEN, JR</u>	ID# <u>3393</u> Date <u>10-01-10</u> ✓
A Agency <u>YAKUTAT DPS</u>	Phone # <u>784-3246</u>
Instrument Location <u>AT POLICE STATION (BOOKING ROOM)</u>	
B Alco S/N <u>77286</u> ✓ Target Value <u>0.082</u> ✓ High Pressure <u>325</u>	
Alco Test Values	<u>0.080</u> ✓ 1st Alco
	<u>0.084</u> ✓ 2nd Alco
Signature	 (OVER)

BMB  
10/5/10

(Do Not write in the area below)


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

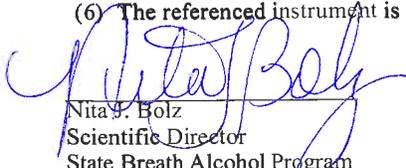  
 Nita J. Bolz  
 Scientific Director  
 State Breath Alcohol Program

Subscribed and sworn before me this 16<sup>th</sup> day of DEC, 2010.

  
 Daniel L. Nicholas  
 Notary Public, State of Alaska  
 Commission Expires with Office



# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N

13ϕ3ϕ3

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130303

OCTOBER 01, 2010

OPERATOR'S NAME:

JENSEN, JAMES I

OPERATOR'S NUMBER: 3393

SUBJECT'S LAST NAME:

UOC

SUBJECT'S FIRST NAME/MI :

U

O.L. #: UOC

DEPT/AGENCY: YAK1

CASE/REPORT: UOC

TEST TYPE: U

ALCO TARGET VALUE: .002

ALCO S/N: 77286

--- BREATH ANALYSIS ---

.002 ADJUSTED FOR 29.65 in  
ALCO TARGET .001 10:00  
BLANK TEST .000 10:00  
INTERNAL STANDARD VERIFIED 10:00  
ALCO TV 29.65 in .000 10:01  
BLANK TEST .000 10:02  
SUBJECT SAMPLE .000 10:02  
BLANK TEST .000 10:03  
ALCO TV 29.65 in .000 10:03  
BLANK TEST .000 10:04

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130303

OCTOBER 01, 2010

TIME 09:56

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 01/08/09

HEATERS

SAMPLE CHAMBER: 49c

BREATH TUBE: 42c

BAROMETER: 29.67 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!@#%&'()\*+,-./0123456789:;<=>?@ABCDEF6  
HIJKLMNPOQRSTUVWXYZ[\]^\_`abcdefgijklmnop  
qrstuvwxyz{|}~||