

# VERIFICATION OF CALIBRATION REPORT

*of DataMaster cdm Breath Test Instrument*

*State of Alaska*

**Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program**

DataMaster cdm S/N: 130305

Supervisor / Operator Performing the Verification Procedure:

Name: William A. Mills ID#: 2688 Date: March 20, 2012

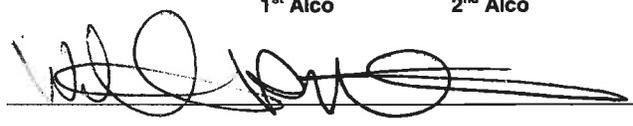
A. Agency: Hoonah Police Department Phone #: 945-3655

Instrument Location: 379 Raven Drive, Hoonah

Alco S/N: 4V Target Value: .080 High Pressure: 1000 psi

B. Alco Test Value Average: .080 .081  
1<sup>st</sup> Alco 2<sup>nd</sup> Alco

Signature

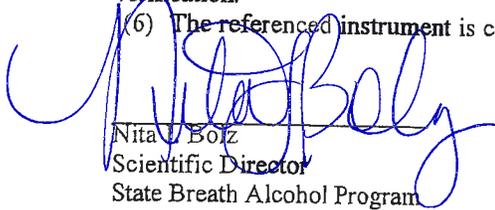


(OVER)


*BMB  
3/30/12*

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 5 day of April, 2012 *(initials)*

 (Notary Seal Stamp)

~~Daniel L. Nicholas~~ *Nikki Roth*  
Notary Public, State of Alaska  
Commission Expires with Office



# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N

130305 <sup>gmb</sup>  
3/30/12

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130305

MARCH 20, 2012

OPERATOR'S NAME: MILLS WILLIAM  
OPERATOR'S NUMBER: 2688  
SUBJECT'S LAST NAME:  
VERIFICATION OF  
SUBJECT'S FIRST NAME/MI :  
CALIBRATION  
O.L. #: 1234567890  
DEPT/AGENCY: HNH1  
CASE/REPORT: 1234567890  
TEST TYPE: U  
ALCO TARGET VALUE: .000  
ALCO S/N: 4U

*BMB 3/30/12*

— BREATH ANALYSIS —

.000 ADJUSTED FOR 29.46 in		
ALCO TARGET	.078	20:21
BLANK TEST	.000	20:22
INTERNAL STANDARD	VERIFIED	20:22
ALCO TV 29.46 in	.000	20:22
BLANK TEST	.000	20:23
SUBJECT SAMPLE	.000	20:24
BLANK TEST	.000	20:24
ALCO TV 29.46 in	.001	20:25
BLANK TEST	.000	20:25

*BMB 3/30/12*

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130305

MARCH 20, 2012  
TIME 20:27

— DIAGNOSTIC CHECK —

COMPUTER:	OKAY
PROGRAM:	OKAY
SOFTWARE DATE:	01/08/09
HEATERS	
SAMPLE CHAMBER:	40c
BREATH TUBE:	41c
BAROMETER:	29.46 in
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

PRINTER TEST  
!"#\$%&'()\*+,-./0123456789:;<=>?@ABCDEF  
GHIJKLMNOPQRSTUVWXYZ[\]^\_`abcdefgijklmno  
pqrstuvwxyz{|}~@