

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130305		
Name	William Mills	ID#	2688	Date	6/12/12
A Agency	Hoonaah Police Department		Phone #	907 945 3655	
Instrument Location	379 Raven Drive, Hoonaah AK 99829				
B Alco S/N	4V	Target Value	.080	High Pressure	850
Alco Test Values	.083	.087	.084	NOB 7/3/12	
	1 <sup>st</sup> Alco	2 <sup>nd</sup> Alco			
Signature					
(OVER)					

(Do Not write in the area below)


BMB  
6/20/12


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 3<sup>rd</sup> day of July 2012. NAK 7/3/12

  
Nikki Roth, Notary Public  
My Commission Expires With Office  
BT9 03/00

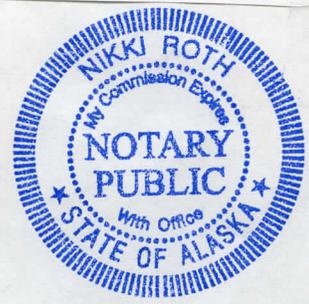

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130305

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130305

JUNE 12, 2012

OPERATOR'S NAME: *BMB 6/20/12*  
NILLS WILLIAM  
OPERATOR'S NUMBER: 2688  
SUBJECT'S LAST NAME:  
VERIFICATION OF  
SUBJECT'S FIRST NAME/MI :  
CALIBRATION  
O.L. #: 123456789  
DEPT/AGENCY: NNH1  
CASE/REPORT: 0987654321  
TEST TYPE: U  
ALCO TARGET VALUE: .080  
ALCO S/N: 4U

### — BREATH ANALYSIS —

.080 ADJUSTED FOR 30.19 in		
ALCO TARGET	.080	00:35
BLANK TEST	.000	00:36
INTERNAL STANDARD	VERIFIED	00:36
ALCO TV 30.19 in	.083	00:37
BLANK TEST	.000	00:37
SUBJECT SAMPLE <i>BMB 6/20/12</i>	.000	00:38
BLANK TEST	.000	00:39
ALCO TV 30.19 in	.084	00:39
BLANK TEST	.000	00:40

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130305

JUNE 12, 2012  
TIME 00:41

### — DIAGNOSTIC CHECK —

COMPUTER:	OKAY
PROGRAM:	OKAY
SOFTWARE DATE:	01/08/09
HEATERS	
SAMPLE CHAMBER:	48c
BREATH TUBE:	42c
BAROMETER:	30.19 in
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

### PRINTER TEST

!"#\$%&'()\*+,-./0123456789:;<=>?@ABCDEF  
GHIJKLMNPOQRSTUVWXYZ[\]^\_`abcdefghijklmnop  
qrstuvwxyz{|}~