

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure: DataMaster cdm S/N 130305

Name ANDRE ACHEE ID# 2385 Date 2/9/2008 ✓

A Agency BETHEL POLICE DEPT Phone # 907-543-3781

Instrument Location Seena

B Alco S/N 78966 Target Value .079 High Pressure 100

Alco Test Values .076 .076
1st Alco 2nd Alco

Supervisor/Operator Performing the Verification Procedure:
Name _____ ID# _____ Date _____
Signature [Signature] A. ACHEE / LT-RPD


Instrument Location _____ (OVER)

Under the Alaska Rules of Evidence, I certify that in the area below)

(a) I am Jeanne Swartz, Criminalist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Andre Achee, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

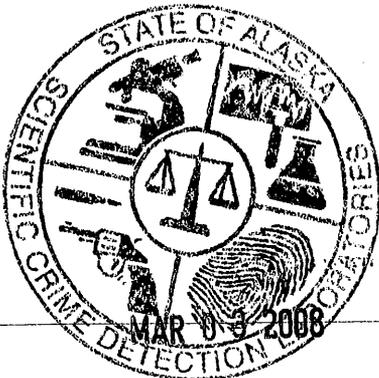

Signed and sealed

[Signature]

03/10/08

Jeanne Swartz
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

Date

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130305

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130305

FEBRUARY 09, 2008

OPERATOR'S NAME:

ACHEE/ANDRE/A

OPERATOR'S NUMBER: 2385

SUBJECT'S LAST NAME:

TEST

SUBJECT'S FIRST NAME/MI :

TEST

O.L. #: 1234567

DEPT/AGENCY: BET1

CASE/REPORT: 000000

TEST TYPE: T

ALCO TARGET VALUE: .078

ALCO S/N: 75566

--- BREATH ANALYSIS ---

.079 ADJUSTED FOR 29.64 in
ALCO TARGET .078 19:07
BLANK TEST .000 19:08
INTERNAL STANDARD VERIFIED 19:08
ALCO TV 29.64 in .076 19:09
BLANK TEST .000 19:10
SUBJECT SAMPLE .000 19:10
BLANK TEST .000 19:11
ALCO TV 29.64 in .076 19:11
BLANK TEST .000 19:12

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130305

FEBRUARY 09, 2008

TIME 19:13

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 02/20/01

HEATERS

SAMPLE CHANGER: 49c

BREATH TUBE: 42c

BAROMETER: 29.64 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

012345678910111213141516171819
ABCDEFGHIJKLMNPQRSTU VWXYZ[*]_ abcdefghijklmnop
qrstuvwxyz{|}~@