

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

JAN 19 2010

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	<u>130305</u>
A	Name	<u>Anthony Wallace</u>	ID# <u>6555</u> Date <u>1/14/10</u>
	Agency	<u>Hoonah Police Department</u>	Phone # <u>945-3655</u>
	Instrument Location	<u>Hoonah Police Department</u>	
B	Alco S/N	<u>2301532</u>	Target Value <u>.082</u> High Pressure <u>800 PSI</u>
	Alco Test Value Average	<u>.084</u>	<u>.087</u>
		1 st Alco	2 nd Alco
Signature		<u>[Signature]</u>	<u>[Signature]</u> 1/29/10
(OVER)			


I, Nita J. Bolz, after being first duly sworn, depose and state as follows in the area below)

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

[Signature]
Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 20th day of January 2010.

[Signature] (Notary Seal Stamp)
Carolyn M. Noland
Notary Public, State of Alaska
Commission Expires with Office

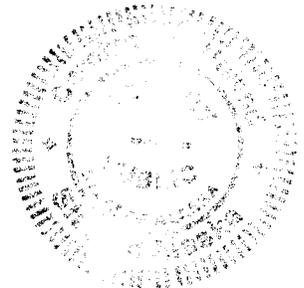

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130505

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130305

JANUARY 14, 2010

OPERATOR'S NAME: WALLACE ANTHONY
OPERATOR'S NUMBER: 6555
SUBJECT'S LAST NAME: UOC

SUBJECT'S FIRST NAME/MI: UOC

O.L. #: UOC
DEPT/AGENCY: HHW1
CASE/REPORT: UOC
TEST TYPE: U

ALCO TARGET VALUE: .002
ALCO S/N: K301532

— BREATH ANALYSIS —

.002 ADJUSTED FOR 29.65 in
ALCO TARGET .001 10:33
BLANK TEST .000 10:34
INTERNAL STANDARD VERIFIED 10:34
ALCO TV 29.67 in .004 10:34
BLANK TEST .000 10:35
SUBJECT SAMPLE .000 10:35
BLANK TEST .000 10:36
ALCO TV 29.67 in .007 10:36
BLANK TEST .000 10:37

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130305

JANUARY 14, 2010
TIME 10:18

— DIAGNOSTIC CHECK —

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 01/08/09

HEATERS
SAMPLE CHAMBER: 48c
BREATH TUBE: 42c

BAROMETER: 29.67 in

FLOW DETECTOR: OKAY

PUMP
HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!*"#%&'()*+,-./0123456789:;<=>?@ABCDEF6
HIJKL MNOPQRSTUVWXYZ[\]^_`abcdefg h i j k l m n o
p q r s t u v w x y z { | } ~