

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program


DataMaster cdm S/N <u>130306</u>	
Supervisor/Operator Performing the Verification Procedure:	
Name <u>STEVE DUNN</u>	ID# <u>4106</u> Date <u>3-18-11</u>
A Agency <u>APD</u>	Phone # <u>786-8900</u>
Instrument Location <u>4th AVE SUB.</u>	
B Alco S/N <u>X124669</u> Target Value <u>.077</u> High Pressure <u>800 PSI</u>	
Alco Test Values <u>.073</u> <u>.074</u>	
1 st Alco 2 nd Alco	
Signature 	
(OVER)	

BMB
4/1/11

(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:


- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

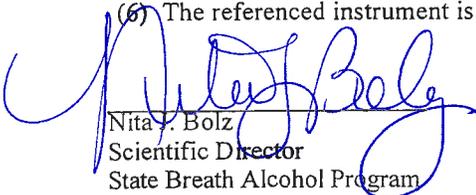
Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 1st day of APRIL, 2010 AN

 (Notary Seal Stamp)

Daniel L. Nicholas
Notary Public, State of Alaska
Commission Expires with Office



VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N **130306**

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

S. Dunn #1361
ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130306

MARCH 18, 2011

OPERATOR'S NAME: *BMB 4/11/11*
DUNN/S
OPERATOR'S NUMBER: 4106
SUBJECT'S LAST NAME:
VERIFICATION OF CAL
SUBJECT'S FIRST NAME/MI :
U

D.L. #: U
DEPT/AGENCY: ANC1
CASE/REPORT: U
TEST TYPE: U
ALCO TARGET VALUE: .077
ALCO S/N: X124659

— BREATH ANALYSIS —

BMB 4/11/11
.077 ADJUSTED FOR 30.24 in
ALCO TARGET .077 10:17
BLANK TEST .000 10:18
INTERNAL STANDARD VERIFIED 10:18
ALCO TV 30.24 in .073 10:18
BLANK TEST .000 10:19
SUBJECT SAMPLE .000 10:21
BLANK TEST .000 10:22
ALCO TV 30.24 in .074 10:22
BLANK TEST .000 10:23

DIAGNOSTIC CHECK

S. Dunn #1361
ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130306

MARCH 18, 2011
TIME 10:10

— DIAGNOSTIC CHECK —

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 02/20/01
HEATERS
SAMPLE CHAMBER: 49c
BREATH TUBE: 43c
BAROMETER: 30.24 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

! " # \$ % & ' () * + , - . / 0 1 2 3 4 5 6 7 8 9 : ; (=) ? @ A B C D E F G
H I J K L M N O P Q R S T U V W X Y Z [\] ^ _ ` a b c d e f g h i j k l m n o
p q r s t u v w x y z { | } ~ ¡ ¢