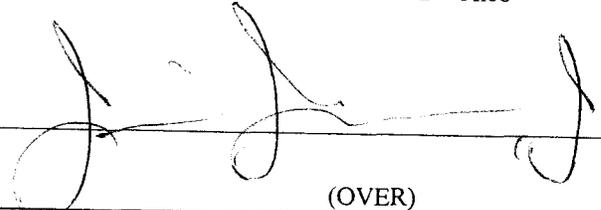


# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument  
State of Alaska

JUL 13 2009

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program


Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	134347 ✓
Name		JAMES I JENSEN, JR	ID# 3393 Date 7/8/09 ✓
A	Agency	YAKUTAT DPS	Phone # 784-3246
Instrument Location		AT POLICE STATION ✓	
B	Alco S/N	77286 ✓	Target Value .482 ✓ High Pressure 854 ✓
Alco Test Values		.483 ✓ 1 <sup>st</sup> Alco	.481 ✓ 2 <sup>nd</sup> Alco
Signature		 ✓	
CRB 7/10/09			

(OVER)


(Do Not write in the area below)


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

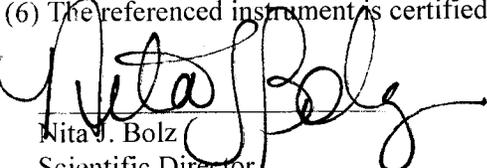  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 21<sup>st</sup> day of Jul, 2009.

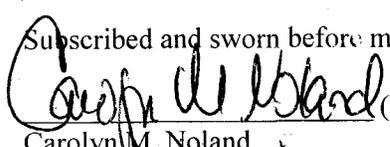  
(Notary Seal Stamp)  
Carolyn M. Noland  
Notary Public, State of Alaska  
Commission Expires with Office



# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 134307 ✓

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130307

JULY 08, 2009 ✓ *CDP #114109*

OPERATOR'S NAME:  
JAMES JENSEN JR  
OPERATOR'S NUMBER: 3393  
SUBJECT'S LAST NAME:  
VOC  
SUBJECT'S FIRST NAME/MI :  
U  
D.L. #: U  
DEPT/AGENCY: YAKI  
CASE/REPORT: U  
TEST TYPE: U ✓  
ALCO TARGET VALUE: .002 ✓  
ALCO S/N: 77286 ✓

### --- BREATH ANALYSIS ---

.002 ADJUSTED FOR 30.33 in  
ALCO TARGET .003 19:07  
BLANK TEST .000 19:08  
INTERNAL STANDARD VERIFIED 19:08  
ALCO TU 30.33 in .003 ✓ 19:08  
BLANK TEST .000 ✓ 19:09  
SUBJECT SAMPLE *CDP #114109* .000 ✓ 19:10  
BLANK TEST .000 ✓ 19:10  
ALCO TU 30.33 in .001 19:11  
BLANK TEST .000 19:12

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130307

JULY 08, 2009 ✓  
TIME 19:04

### --- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 02/20/01  
HEATERS  
SAMPLE CHAMBER: 50c  
BREATH TUBE: 40c  
BAROMETER: 30.33 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

### PRINTER TEST

!""#%&'()\*+,-./0123456789:;<=>?@ABCDEF  
GHIJKLMNOPQRSTUVWXYZ[\]^\_`abcde fghijklmno  
pqrstuvwxyz{|}~■