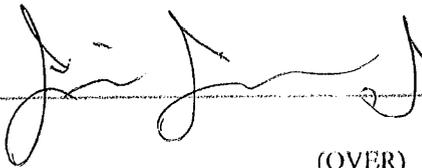


VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130347 ✓			
Name	JAMES I JENSEN, JR	ID#	3393	Date	11 AUG 08 ✓	
A	Agency	YAKUTAT DPS ✓	Phone #	784-3246		
Instrument Location	AT POLICE STATION ✓					
B	Alco S/N	X301586 ✓	Target Value	.077 ✓	High Pressure	700
Alco Test Value Average	.078 ✓	.078 ✓				
	1 st Alco	2 nd Alco				
Signature				CS 8/18/08		
(OVER)						

(Do Not write in the area below)


Under the Alaska Rules of Evidence, I certify that;


(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, James I Jensen, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed,

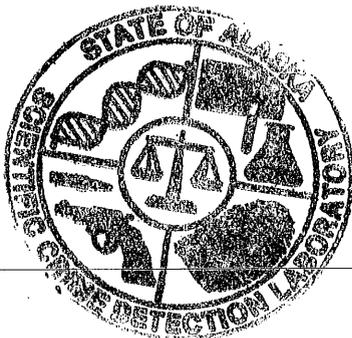



Jeanne Swartz
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

8/20/08

Date

BT9 03/00

AUG 14 2008

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130307

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130307

AUGUST 11, 2008

OPERATOR'S NAME:
JENSEN, JAMES I

OPERATOR'S NUMBER: 3393

SUBJECT'S LAST NAME:

UJC

SUBJECT'S FIRST NAME/MI:

L

O.L. #: L

DEPT/AGENCY: YAK1

CASE/REPORT:

TEST TYPE: V

ALCO TARGET VALUE: .077

ALCO S/N: X301586

--- BREATH ANALYSIS ---

.077 ADJUSTED FOR 30.32 in
ALCO TARGET .078 01:56
BLANK TEST .000 01:57
INTERNAL STANDARD VERIFIED 01:57
ALCO TV 30.32 in .078 01:57
BLANK TEST .000 01:58
SUBJECT SAMPLE .000 01:59
BLANK TEST .000 02:00
ALCO TV 30.32 in .078 02:00
BLANK TEST .000 02:01

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130307

AUGUST 11, 2008

TIME 01:52

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 02/20/01

HEATERS

SAMPLE CHAMBER: 51c

BREATH TUBE: 42c

BAROMETER: 30.32 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

! " # % & ' () * + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G
H I J K L M N O P Q R S T U V W X Y Z [\] ^ _ ` a b c d e f g h i j k l m n o
p q r s t u v w x y z { | } ~ #