

APR 01 2011

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure: DataMaster cdm S/N 130308


Name Malik Jones ID# 5830 Date 3/18/11

A Agency AST Phone # 451-5100

Instrument Location NEENANA

B Alco S/N X124655 Target Value .081 High Pressure 700 PST

Alco Test Values .077 .077
 1st Alco 2nd Alco

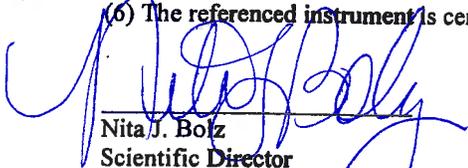
Signature 

(OVER) 


(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


 Nita J. Bolz
 Scientific Director
 State Breath Alcohol Program

Subscribed and sworn before me this 1st day of APRIL, 2011.

 (Notary Seal Stamp)
 Carolyn M. Notland DANIEL L. NICHOLAS
 Notary Public, State of Alaska
 Commission Expires with Office



VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130308

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130308

MARCH 18, 2011

OPERATOR'S NAME: *BMB 4/1/11*
JONES/MALIK/JAMAL
OPERATOR'S NUMBER: 5830
SUBJECT'S LAST NAME:
VERIFICATION OF CAL
SUBJECT'S FIRST NAME/NI :
U

D.L. #: 1
DEPT/AGENCY: HLYB
CASE/REPORT:
TEST TYPE: U
ALCO TARGET VALUE: .081
ALCO S/N: X124655

--- BREATH ANALYSIS ---

.081 ADJUSTED FOR 28.69 in		
ALCO TARGET	.077	14:19
BLANK TEST	.000	14:21
INTERNAL STANDARD	VERIFIED	14:21
ALCO TU 28.69 in	.077	14:21
BLANK TEST	.000	14:22
SUBJECT SAMPLE	.080	14:23
BLANK TEST	.000	14:23
ALCO TU 28.69 in	.077	14:24
BLANK TEST	.000	14:24

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130308

MARCH 18, 2011
TIME 14:26

--- DIAGNOSTIC CHECK ---

COMPUTER:	OKAY
PROGRAM:	OKAY
SOFTWARE DATE:	02/20/01
HEATERS	
SAMPLE CHAMBER:	43c
BREATH TUBE:	43c
BAROMETER:	28.69 in
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

PRINTER TEST

!@#%&'()*+,-./0123456789:;<=>?@ABCDEFG
HIJKLMNOPQRSTUVWXYZ[\]^_`abcdefgijklmnop
qrstuvwxy{|}~