

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N <u>130309</u> ✓
Name	<u>PATRICK NELSON</u>	ID# <u>4389</u> Date <u>3/19/08</u> ✓
A Agency	<u>AST</u>	Phone # <u>373-8337</u>
Instrument Location <u>NATSON WEST</u>		
B Alco S/N	<u>X172971</u> ✓	Target Value <u>.079</u> ✓ High Pressure <u>900</u>
Alco Test Values	<u>.078</u> 1 st Alco	<u>.078</u> 2 nd Alco
Signature	<u>[Signature]</u>	<u>CWS</u> <u>3/25/08</u>


(OVER)

Under the Alaska Rules of Evidence, I certify that (in the area below)

(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Patrick Nelson, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

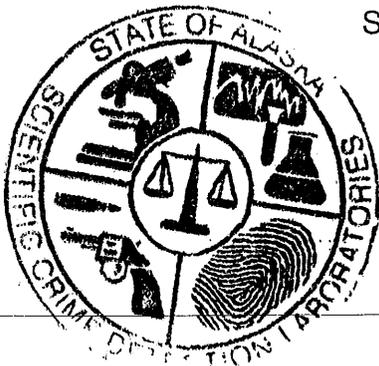

Signed and sealed,

[Signature] 3/26/08
Date
Jeanne Swartz
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130309

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130309

MARCH 19, 2008 *CAS 3/25/08*

OPERATOR'S NAME: NELSON PATRICK
OPERATOR'S NUMBER: 4389
SUBJECT'S LAST NAME:
VERIFICATION OF
SUBJECT'S FIRST NAME/MI :
CALIBRATION
O.L. #: 12345
DEPT/AGENCY: PLM0
CASE/REPORT: 12-3456
TEST TYPE: U
ALCO TARGET VALUE: .079
ALCO S/N: K172977

--- BREATH ANALYSIS ---

.079 ADJUSTED FOR 29.47 in		
ALCO TARGET	.077	20:13
BLANK TEST	.000	20:14
INTERNAL STANDARD	VERIFIED	20:14
ALCO TV 29.47 in	.078	20:15
BLANK TEST	.000	20:15
SUBJECT SAMPLE	.000 <i>CAS 3/25/08</i>	20:16
BLANK TEST	.000	20:17
ALCO TV 29.47 in	.078	20:17
BLANK TEST	.000	20:18

NEW PRINTER

RIBBON INSTALLED *

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130309

MARCH 19, 2008
TIME 20:21

--- DIAGNOSTIC CHECK ---

COMPUTER:	OKAY
PROGRAM:	OKAY
SOFTWARE DATE:	02/20/01
HEATERS	
SAMPLE CHAMBER:	49c
BREATH TUBE:	43c
BAROMETER:	29.47 in
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

PRINTER TEST

! " # \$ % & ' () * + , - . / 0 1 2 3 4 5 6 7 8 9 : ; (=) ? @ A B C D E F G
H I J K L M N O P Q R S T U V W X Y Z [\] ^ _ ` a b c d e f g h i j k l m n o
p q r s t u v w x y z { | } ~