

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument
State of Alaska

JUL 27 2009

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N <u>130309</u>
Name	<u>P. NELSON</u>	ID# <u>4389</u> Date <u>7-21-09</u>
A Agency	<u>AST</u>	Phone # <u>373-8337</u>
Instrument Location	<u>MSW</u>	
Alco S/N <u>70729</u>		Target Value <u>.082</u> High Pressure <u>400</u>
B Alco Test Values	<u>.082</u> ✓ 1 st Alco	<u>.082</u> ✓ 2 nd Alco
Signature	<u>[Signature]</u>	<u>CMB</u> <u>7/30/09</u>

(OVER)


(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

[Signature]
Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 7th day of Aug, 2009.
[Signature] (Notary Seal Stamp)
Carolyn M. Noland
Notary Public, State of Alaska
Commission Expires with Office

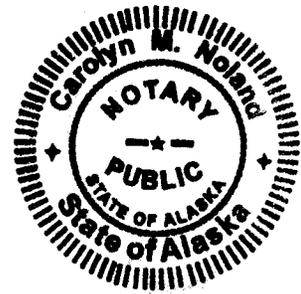

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130309

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130309

JULY 21, 2009 ✓
CDP #130309

OPERATOR'S NAME:
NELSON PATRICK
OPERATOR'S NUMBER: 4389
SUBJECT'S LAST NAME:
VERIFICATION OF
SUBJECT'S FIRST NAME/NI :
CALIBRATION
D.L. #: 123456
DEPT/AGENCY: PL100
CASE/REPORT: 12-3456
TEST TYPE: U
ALCO TARGET VALUE: .062 ✓
ALCO S/N: 70729 ✓

--- BREATH ANALYSIS ---

.062 ADJUSTED FOR 29.75 in		
ALCO TARGET	.061	01:14
BLANK TEST	.000	01:15
INTERNAL STANDARD	VERIFIED	01:15
ALCO TV 29.75 in	.062 ✓	01:15
BLANK TEST	.000 ✓	01:16
SUBJECT SAMPLE	.000 ✓	01:17
BLANK TEST	.000 ✓	01:18
ALCO TV 29.75 in	.062 ✓	01:18
BLANK TEST	.000	01:19

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130309

JULY 21, 2009 ✓
TIME 01:12

--- DIAGNOSTIC CHECK ---

COMPUTER:	OKAY
PROGRAM:	OKAY
SOFTWARE DATE:	02/28/01
HEATERS	
SAMPLE CHAMBER:	49c
BREATH TUBE:	41c
BAROMETER:	29.75 in
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

PRINTER TEST

! " # \$ % & ' () * + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G
H I J K L M N O P Q R S T U V W X Y Z \] ^ _ ` a b c d e f g h i j k l m n o
p q r s t u v w x y z { | } ~ ¡ ¢ £ ¤ ¥ ¦ § ¨ © ª « ¬ ® ¯ ° ± ² ³ ´ µ ¶ · ¸ ¹ º » ¼ ½ ¾