

# VERIFICATION OF CALIBRATION REPORT

of DataMaster edm Breath Test Instrument  
State of Alaska

NOV 23 2009

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

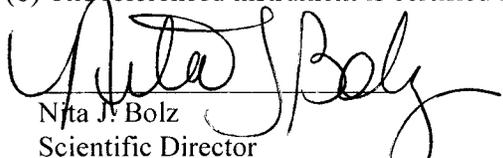
Supervisor/Operator Performing the Verification Procedure:		DataMaster edm S/N <u>130309</u> ✓	
Name	<u>Peter Steen</u>	ID#	<u>4572</u> Date <u>11/19/09</u> ✓
A Agency	<u>AST 1 BHP</u>	Phone #	<u>373-8342</u>
Instrument Location	<u>Mat su west</u> ✓		
B Alco S/N	<u>31085</u> ✓	Target Value	<u>.082</u> ✓ High Pressure <u>900</u>
Alco Test Values	<u>.083</u> ✓ 1 <sup>st</sup> Alco	<u>.084</u> ✓ 2 <sup>nd</sup> Alco	
Signature	 ✓		
(OVER)			

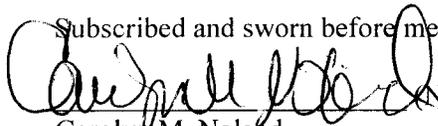
8MB  
12/31/09

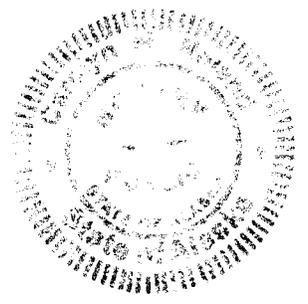
(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 31<sup>st</sup> day of Dec., 2009.  
 (Notary Seal Stamp)  
Carolyn M. Noland  
Notary Public, State of Alaska  
Commission Expires with Office



# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130309 ✓

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130309

NOVEMBER 19, 2009

OPERATOR'S NAME:

STEEN, PETER, C

OPERATOR'S NUMBER: 4572

SUBJECT'S LAST NAME:

UOC

SUBJECT'S FIRST NAME/MI :

UOC

O.L. #: UOC

DEPT/AGENCY: PALT

CASE/REPORT: UOC

TEST TYPE: U

ALCO TARGET VALUE: .002 ✓

ALCO S/N: 31005 ✓

### — BREATH ANALYSIS —

.002 ADJUSTED FOR 29.49 in ✓

ALCO TARGET	.000	17:14
BLANK TEST	.000	17:15
INTERNAL STANDARD	VERIFIED	17:15
ALCO TU 29.49 in	.003 ✓	17:15
BLANK TEST	.000	17:16
SUBJECT SAMPLE	.000	17:17
BLANK TEST	.000	17:17
ALCO TU 29.49 in	.004	17:18
BLANK TEST	.000	17:19

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130309

NOVEMBER 19, 2009 ✓  
TIME 17:12

### — DIAGNOSTIC CHECK —

COMPUTER:	OKAY
PROGRAM:	OKAY
SOFTWARE DATE:	02/28/01
HEATERS	
SAMPLE CHAMBER:	49c
BREATH TUBE:	41c
BAROMETER:	29.49 in
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

### PRINTER TEST

!"#\$%&'()\*+,-./0123456789:;<=>?@ABCDEFGHIJKL  
MNOPQRSTUVWXYZ[\]^\_`abcdefghijklmnopqrstuvwxyz{|}~  
!@#\$%^&\*()~