

**VERIFICATION OF CALIBRATION REPORT**  
*of DataMaster cdm Breath Test Instrument*  
*State of Alaska*  
*Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program*

DataMaster cdm S/N <u>130309<sup>✓</sup></u>	
Supervisor/Operator Performing the Verification Procedure:	
Name <u>PATRICK NELSON</u>	ID# <u>4389<sup>✓</sup></u> Date <u>11/21/10<sup>✓</sup></u>
A Agency <u>AST</u> Phone # <u>746-9108</u>	
Instrument Location <u>MATSU WEST AST</u>	
B Alco S/N <u>X301599<sup>✓</sup></u> Target Value <u>.082<sup>✓</sup></u> High Pressure <u>500</u>	
Alco Test Values	<u>.084<sup>✓</sup></u> <u>.084<sup>✓</sup></u>
	1 <sup>st</sup> Alco 2 <sup>nd</sup> Alco
Signature <u>[Signature]</u>	
(OVER)	

*BMB  
12/16/10*


- I, Nita J. Bolz, after being first duly sworn, depose and state as follows. (Do Not write in the area below)
- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
  - (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
  - (3) I am the Scientific Director of the State Breath Alcohol Program.
  - (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
  - (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
  - (6) The **referenced** instrument is certified for evidentiary use in the State of Alaska.

[Signature]  
 Nita J. Bolz  
 Scientific Director  
 State Breath Alcohol Program

Subscribed and sworn before me this 23<sup>RD</sup> day of DEC, 2010.

[Signature] (Notary Seal Stamp)

Daniel L. Nicholas  
 Notary Public, State of Alaska  
 Commission Expires with Office

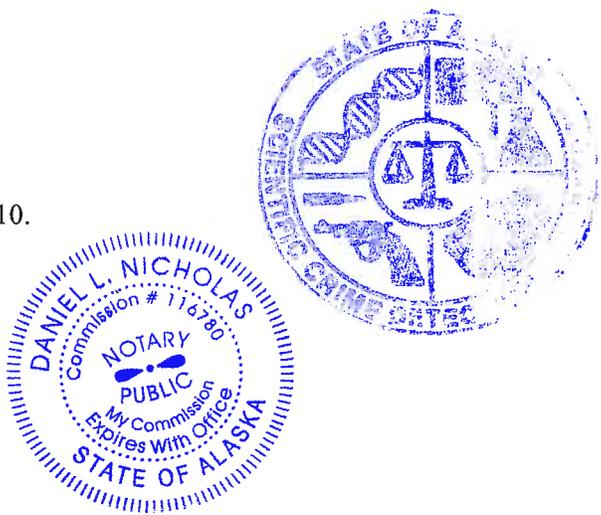

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130309 <sup>DLW</sup> <sub>12/19/10</sub>

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130309

NOVEMBER 21, 2010

OPERATOR'S NAME:  
NELSON PATRICK  
OPERATOR'S NUMBER: 4309  
SUBJECT'S LAST NAME:

VERIFICATION OF  
SUBJECT'S FIRST NAME/MI :

CALIBRATION

O.L. #: 123456  
DEPT/AGENCY: PLM0  
CASE/REPORT: 12-3456  
TEST TYPE: U  
ALCO TARGET VALUE: .002  
ALCO S/N: X301599

### --- BREATH ANALYSIS ---

.002 ADJUSTED FOR 30.14 in  
ALCO TARGET .002 09:49  
BLANK TEST .000 09:50  
INTERNAL STANDARD VERIFIED 09:50  
ALCO TV 30.14 in .004 09:51  
BLANK TEST .000 09:52  
SUBJECT SAMPLE .000 09:53  
BLANK TEST .000 09:53  
ALCO TV 30.14 in .004 09:54  
BLANK TEST .000 09:55

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130309

NOVEMBER 21, 2010  
TIME 09:55

### --- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 02/20/01  
HEATERS  
SAMPLE CHAMBER: 49c  
BREATH TUBE: 40c  
BAROMETER: 30.14 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

### PRINTER TEST

!@#&'()\*+,-./0123456789:;<=>?@BCDEFG  
HIJKL MNOPQRSTUVWXYZ[\]^\_`abcde fghijklmno  
pqrstuvwxyz{|}~||