

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	<u>130404</u>
Name		<u>BRAD REED</u>	ID# <u>6158</u> Date <u>26 July 2008</u> ✓
A	Agency	<u>FORT Greely Police Department</u> ✓	Phone # <u>907-873-9149</u>
Instrument Location		<u>Booking Room</u>	
Alco S/N		<u>X124625</u> ✓	Target Value <u>.080</u> ✓ High Pressure <u>500psi</u>
Alco Test Values		<u>.079</u> ✓ 1 st Alco	<u>.079</u> ✓ 2 nd Alco
Signature		<u>[Signature]</u>	<u>CS</u> <u>8/12/08</u>

(OVER)


Under the Alaska Rules of Evidence, I certify that, ^(Do Not write in the area below)

(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Brad G Reed, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed,

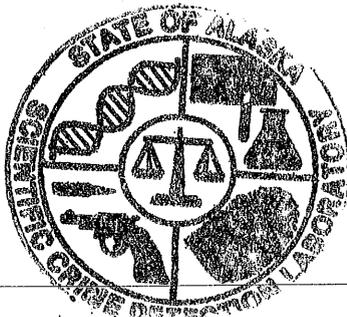

[Signature]

Jeanne Swartz
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

8/13/08
Date

AUG 01 2008

BT9 06/03

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130404 ✓

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130404

JULY 26, 2008 *CAS 8/2/08*

OPERATOR'S NAME:

REED/BRAD/G

OPERATOR'S NUMBER: 6158

SUBJECT'S LAST NAME:

VOC

SUBJECT'S FIRST NAME/MI :

VOC

O.L. #: VOC

DEPT/AGENCY: B164

CASE/REPORT: VOC

TEST TYPE: V

ALCO TARGET VALUE: .000 ✓

ALCO S/N: X124625 ✓

--- BREATH ANALYSIS ---

.000 ADJUSTED FOR 28.50 in
ALCO TARGET .076 12:24
BLANK TEST .000 12:25
INTERNAL STANDARD VERIFIED 12:25
ALCO TV 28.50 in .079 ✓ 12:25
BLANK TEST .000 12:26
SUBJECT SAMPLE .000 *CAS 8/2/08* 12:27
BLANK TEST .000 12:27
ALCO TV 28.50 in .079 ✓ 12:28
BLANK TEST .000 12:29

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130404

JULY 26, 2008 ✓

TIME 12:28

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 02/20/01

HEATERS

SAMPLE CHAMBER: 48c

BREATH TUBE: 40c

BAROMETER: 28.50 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!"#\$%&'()*+,-./0123456789:;<=>@ABCDEFGHIJKL
MNPQRSTUVWXYZ[\]^_`abcde fghijklmno
pqrstuvwxyz{|}~