

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

JUL 13 2010

State of Alaska

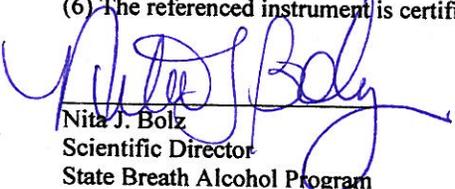
Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130404 ✓
Name	John Carroll ✓	ID#	6775 ✓
Date	July 7 2010 ✓		
A Agency	Fort Greely Police Dept. BIG4		Phone # 907-873-9120
Instrument Location	Bldg. 663, Fort Greely Police Booking Room		
B Alco S/N	X172958 ✓	Target Value	.087 ✓
High Pressure	800		
Alco Test Values	.085 ✓	.085 ✓	
	1 <sup>st</sup> Alco	2 <sup>nd</sup> Alco	
Signature			COB 7/15/10
(OVER)			

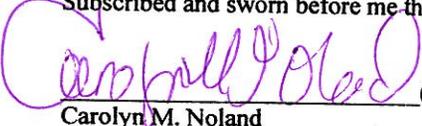
(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 27<sup>th</sup> day of July, 2010.

  
Carolyn M. Noland  
Notary Public, State of Alaska  
Commission Expires with Office

(Notary Seal Stamp)

BT9 06/03



# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130404

(CONTINUED FROM FRONT PAGE)

**C** TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130404

JULY 07, 2010

OPERATOR'S NAME:

CARROLL, JOHN

OPERATOR'S NUMBER: 6775

SUBJECT'S LAST NAME:

VOC

SUBJECT'S FIRST NAME/MI :

VOC

O.L. #: 000000

DEPT/AGENCY: FT GREELY PD B164

CASE/REPORT: 10-0000

TEST TYPE: V

ALCO TARGET VALUE: .087

ALCO S/N: X172953

--- BREATH ANALYSIS ---

.087 ADJUSTED FOR 28.92 in  
ALCO TARGET .084 20:44  
BLANK TEST .000 20:45  
INTERNAL STANDARD VERIFIED 20:45  
ALCO TV 28.92 in .085 20:46  
BLANK TEST .000 20:46  
SUBJECT SAMPLE .000 20:47  
BLANK TEST .000 20:48  
ALCO TV 28.92 in .085 20:48  
BLANK TEST .000 20:49

## DIAGNOSTIC CHECK:

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130404

JULY 07, 2010

TIME 20:41

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 01/08/09

HEATERS

SAMPLE CHAMBER: 48c

BREATH TUBE: 41c

BAROMETER: 28.92 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!""#%&'()\*+,-./0123456789:;<=>?@ABCDEFGHIJ  
KLMNOPQRSTUVWXYZ[\]^\_`abcdefgijklmnop  
qrstuvwxyz{|}~`