

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:  
Name Shayne Calt ID# 4559 Date 1-24-09 ✓  
DataMaster cdm S/N 130492 ✓

A. Agency AST Phone # 733-2256  
Instrument Location Willow AST ✓

B. Alco S/N 75470 ✓ Target Value .076 ✓ High Pressure 500  
Alco Test Value Average .079 ✓ .078 ✓  
1<sup>st</sup> Alco 2<sup>nd</sup> Alco

Signature [Signature] ✓ [Signature] ✓  
Date 3/1/09 ✓


Under the Alaska Rules of Evidence, I certify that: (OVER)

(a) I am Jeanne Swartz, Forensic Scientist II, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Shayne M Calt, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed,

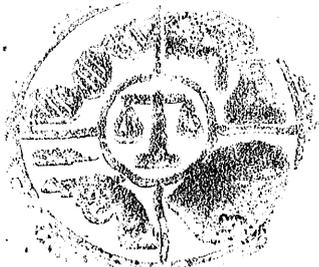

[Signature] 3/2/09  
Date  
Jeanne Swartz  
Scientific Director Designee  
State of Alaska  
State Breath Alcohol Testing Program

FEB 24 2009

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130492

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130492

JANUARY 24, 2009

OPERATOR'S NAME:  
CALT SHAYNE H  
OPERATOR'S NUMBER: 4559  
SUBJECT'S LAST NAME:  
VERIFICATION OF CAL  
SUBJECT'S FIRST NAME/MI :  
V

O.L. #: V  
DEPT/AGENCY: TALO  
CASE/REPORT: V  
TEST TYPE: V  
ALCO TARGET VALUE: .076 ✓  
ALCO S/N: 75470 ✓

--- BREATH ANALYSIS ---

.076 ADJUSTED FOR 30.25 in		
ALCO TARGET	.076	17:38
BLANK TEST	.000	17:39
INTERNAL STANDARD	VERIFIED	17:39
ALCO TV 30.25 in	.079 ✓	17:40
BLANK TEST	.000	17:40
SUBJECT SAMPLE	.000	17:41
BLANK TEST	.000	17:42
ALCO TV 30.25 in	.078 ✓	17:42
BLANK TEST	.000	17:43

BT9 03/00

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130492

JANUARY 24, 2009  
TIME 17:36

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 02/20/01  
HEATERS  
SAMPLE CHAMBER: 49c  
BREATH TUBE: 41c  
BAROMETER: 30.25 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

PRINTER TEST

!"#\$%&'()\*+,-./0123456789:;<=?@ABCDEF6  
HIJKLMNPQRSTUWXYZ\]^\_`abcde-fghi.jklmno  
pqrstuvwxyz{|}~