


VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument
State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130492
Name	Shayne Calt	ID#	4559
		Date	3/22/08 ✓ CSB
A	Agency	AST	Phone # 733-2256
	Instrument Location	Willow AST	
B	Alco S/N	X301755 ✓	Target Value .079 ✓
			High Pressure 300
	Alco Test Value Average	.080	.080
		1 st Alco	2 nd Alco
	Signature		CSB 3/25/08


(OVER)

Under the Alaska Rules of Evidence, I certify that;


(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Shayne M Calt, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

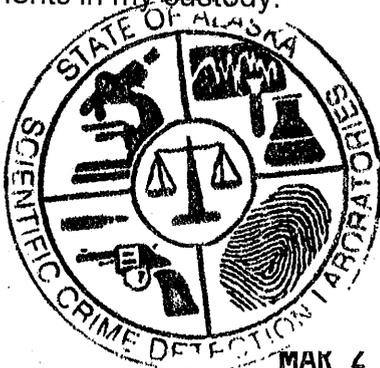

Signed and sealed,



Jeanne Swartz
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

3/26/08
Date

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130492

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130492

MARCH 22, 2008

OPERATOR'S NAME: *CAS 3/26/08*
CALT SHAYNE H
OPERATOR'S NUMBER: 4553
SUBJECT'S LAST NAME:
VERIFICATION CODE:
SUBJECT'S FIRST NAME/MI :
A
A.L. #: A
DEPT/AGENCY: TALA
CASE/REPORT: A
TEST TYPE: V
ALCO TARGET VALUE: .079
ALCO S/N: X301755

--- BREATH ANALYSIS ---

.079 ADJUSTED FOR 29.47 in
ALCO TARGET .077 18:09
BLANK TEST .000 18:11
INTERNAL STANDARD VERIFIED 18:11
ALCO TV 29.47 in .000 18:11
BLANK TEST .000 18:12
SUBJECT SAMPLE .000 *CAS 3/26/08* 18:12
BLANK TEST .000 18:13
ALCO TV 29.47 in .000 18:14
BLANK TEST .000 18:14

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130492

MARCH 22, 2008
TIME 18:16

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 02/26/01
HEATERS
SAMPLE CHAMBER: 49c
BREATH TUBE: 41c
BAROMETER: 29.47 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

!@#%&'()*+,-./0123456789:;<=>?@ABCDEF6
HIJKLMNOPQRSTUVWXYZ[\]^_`abcde fghijklmnop
qrstuvwxy{|}~`