


VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130492			
Name	Shayne Calt	ID#	4559	Date	7-18-08 ✓	
A	Agency	AST	Phone #	733-2258		
Instrument Location		Willow ✓				
Alco S/N		75470 ✓	Target Value	.076 ✓	High Pressure	800 psi
B		Alco Test Value Average	.076 ✓	.075 ✓		
		1 st Alco	2 nd Alco			
Signature				JCS 8/28/08		


Under the Alaska Rules of Evidence, I certify that; (OVER)


(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Shayne M Calt, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed,

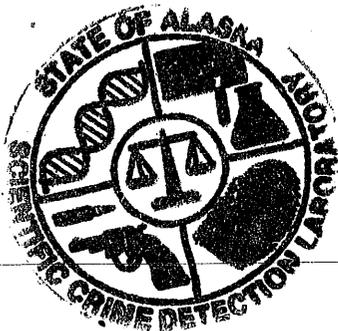



Jeanne Swartz
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

08/28/08

Date

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130492 V

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130492

JULY 16, 2008 ✓ *DOB 8/28/08*

OPERATOR'S NAME:
CALT SHAYNE H
OPERATOR'S NUMBER: 4559
SUBJECT'S LAST NAME:
VERIFICATION/FINAL
SUBJECT'S FIRST NAME/MI :
V
O.L. #: V
DEPT/AGENCY: TALO
CASE/REPORT: V
TEST TYPE: V
ALCO TARGET VALUE: .076 ✓
ALCO S/N: 75470 ✓

--- BREATH ANALYSIS ---

.076 ADJUSTED FOR 29.65 in
ALCO TARGET .075 06:36
BLANK TEST .000 06:37
INTERNAL STANDARD VERIFIED 06:37
ALCO TV 29.65 in .076 ✓ 06:37
BLANK TEST .000 06:38
SUBJECT SAMPLE .000 *DOB 8/28/08* 06:39
BLANK TEST .000 06:39
ALCO TV 29.65 in .075 ✓ 06:40
BLANK TEST .000 06:40

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130492

JULY 16, 2008 ✓
TIME 06:31

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 02/20/01
HEATERS
SAMPLE CHAMBER: 49c
BREATH TUBE: 41c
BAROMETER: 29.65 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

1"#\$%&'()*+,-./0123456789:;<=>@ABCDEF
"###NPNORSTUVWXYZ[]_`abcde/ghijklmno
pqrstuvwxy{|~?@