

VERIFICATION OF CALIBRATION REPORT

JAN 20 2010

of Datamaster cdm
State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

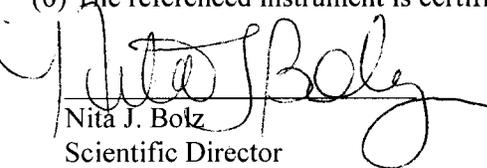
Supervisor/Operator Performing the Verification Procedure:		Datamaster cdm S/N <u>130492</u>	
Name	<u>Shayne Calt</u>	ID#	<u>4559</u> Date <u>11-24-09</u>
A Agency	<u>AST</u>	Phone #	<u>733-2256</u>
Instrument Location	<u>Willow AST</u>		
B Alco S/N	<u>X301581</u>	Target Value	<u>.082</u> High Pressure <u>1000</u>
Alco Test Value Average	<u>.082</u> 1 st Alco	<u>.081</u> 2 nd Alco	
Signature			<u>CBS</u> <u>1/20/10</u>

(OVER)

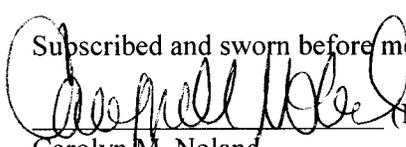
(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 26th day of January 2010.


(Notary Seal Stamp)
Carolyn M. Noland
Notary Public, State of Alaska
Commission Expires with Office



VERIFICATION OF CALIBRATION REPORT

of Datamaster cdm

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Datamaster cdm S/N

130492

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130492

NOVEMBER 24, 2009

OPERATOR'S NAME:

DALE SHAYNE M

OPERATOR'S NUMBER: 4559

SUBJECT'S LAST NAME:

VERIFICATION OF CAL

SUBJECT'S FIRST NAME/MI:

V

O.L. #: V

DEPT/AGENCY: TAL0

CASE/REPORT: V

TEST TYPE: V

ALCO TARGET VALUE: .002

ALCO S/N: 130492

X301581

--- BREATH ANALYSIS ---

.002 ADJUSTED FOR 29.38 in		
ALCO TARGET	.000	20:26
BLANK TEST	.000	20:27
INTERNAL STANDARD	VERIFIED	20:27
ALCO TV 29.38 in	.002	20:27
BLANK TEST	.000	20:28
SUBJECT SAMPLE	.000	20:29
BLANK TEST	.000	20:29
ALCO TV 29.38 in	.001	20:30
BLANK TEST	.000	20:30

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130492

NOVEMBER 24, 2009

TIME 20:23

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 02/20/01

HEATERS

SAMPLE CHAMBER: 49c

BREATH TUBE: 41c

BAROMETER: 29.38 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!@#%&'()*+,-./0123456789:;<=>?@ABCDEF6
HIJKLMNPQRSTUWXYZ[\]^_`abcde(ghijklmno
pqrstuvwxyz{|}~