

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument  
State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

		DataMaster cdm S/N	180493	
Supervisor/Operator Performing the Verification Procedure:		3/3/12 <sup>BMB</sup> 3/4/12 BMB 4/3/12		
Name	Ronny Simmons	ID #	5123	
Date:	3-4-12			
A Agency	AST	Phone #	320-6166	
Instrument Location	Clear Air Force Station			
Alco S/N	X124609	Target Value	.081	
High Pressure	1050			
B Alco Test Values	1st Alco	.077	2nd Alco	.078
Signature	 RAS			

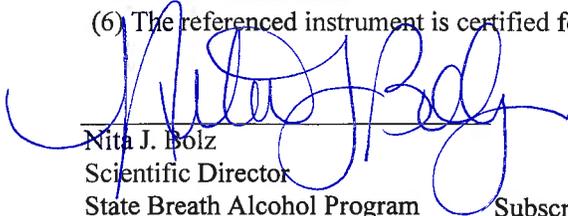
(OVER)

BMB  
4/3/12


(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and states as follows:

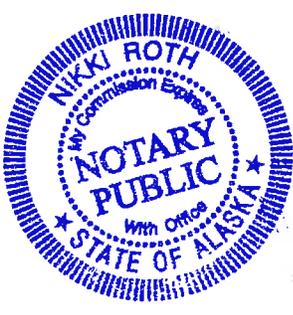
- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 5 day of April, 2012 4/5/12

  
Daniel L. Nicholas  
Notary Public, State of Alaska  
Commission Expires with Office

 (Notary Seal Stamp)



# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument  
State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130493

(CONTINUED FROM FRONT PAGE)

**C** TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT AND THE TEST DIAGNOSTIC CHECK THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130493

MARCH 03, 2012

OPERATOR'S NAME: SIMMONSRONNYA  
*BOMB 4/13/12*

OPERATOR'S NUMBER: 5123  
SUBJECT'S LAST NAME: VERIFICATION/FICAL  
SUBJECT'S FIRST NAME/MI: S

O.L. #: 1  
DEPT/AGENCY: CLR4  
CASE/REPORT: 1  
TEST TYPE: V  
ALCO TARGET VALUE: .081  
ALCO S/N: X124609

--- BREATH ANALYSIS ---

.081 ADJUSTED FOR 29.49 in		
ALCO TARGET	.079	12:58
BLANK TEST	.000	12:59
INTERNAL STANDARD	VERIFIED	12:59
ALCO TV 29.49 in	.077	12:59
BLANK TEST	.000	13:00
SUBJECT SAMPLE	.000	13:01
BLANK TEST	.000	13:01
ALCO TV 29.49 in	.078	13:02
BLANK TEST	.000	13:02

*BOMB 4/13/12*

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130493

MARCH 03, 2012  
TIME 13:03

--- DIAGNOSTIC CHECK ---

COMPUTER:	OKAY
PROGRAM:	OKAY
SOFTWARE DATE:	01/00/09
HEATERS	
SAMPLE CHAMBER:	49c
BREATH TUBE:	42c
BAROMETER:	29.49 in
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

PRINTER TEST

!@%&'()\*+,-./0123456789:;<=>?@ABCDEF6  
HIJKLMNOPQRSTUVWXYZ\*~\_ ' abcdefghijklmnop  
pqrstuvwxyz{|}~+\*

