


# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

AUG 05 2009

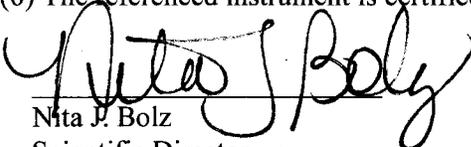
Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N <u>130493</u> ✓
Name	<u>PATRICK J. SMITH</u>	ID# <u>6397</u> Date <u>27 JUL 2009</u> ✓
A Agency	<u>CLEAR SECURITY FORCES</u>	Phone # <u>907-585-6293</u>
Instrument Location	<u>Bldg 37, Clear Air Force Station, AK</u> ✓	
B Alco S/N	<u>X124609</u> ✓	Target Value <u>.081</u> ✓ High Pressure <u>1200</u>
Alco Test Values	<u>.075</u> ✓ 1 <sup>st</sup> Alco	<u>.076</u> ✓ 2 <sup>nd</sup> Alco
Signature		 8/11/09

(OVER)

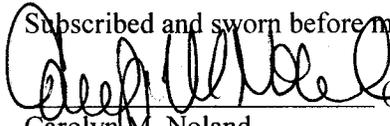
(Do Not write in the area below)


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 14<sup>th</sup> day of August, 2009.

  
(Notary Seal Stamp)  
Carolyn M. Noland  
Notary Public, State of Alaska  
Commission Expires with Office



# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130493

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130493

JULY 27, 2009 ✓

OPERATOR'S NAME:  
SMITH/PATRICK/J  
OPERATOR'S NUMBER: 6397  
SUBJECT'S LAST NAME:  
VOC

SUBJECT'S FIRST NAME/MI :  
VOC

O.L. #: 1234567  
DEPT/AGENCY: CLR4  
CASE/REPORT: 20090727  
TEST TYPE: V  
ALCO TARGET VALUE: .081 ✓  
ALCO S/N: X124609 ✓

### --- BREATH ANALYSIS ---

.081 ADJUSTED FOR 29.65 in  
ALCO TARGET .080 15:19  
BLANK TEST .000 15:20  
INTERNAL STANDARD VERIFIED 15:20  
ALCO TV 29.65 in .075 ✓ 15:20  
BLANK TEST .000 15:21  
SUBJECT SAMPLE .000 15:21  
BLANK TEST .000 15:22  
ALCO TV 29.65 in .076 ✓ 15:22  
BLANK TEST .000 15:23

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130493

JULY 27, 2009 ✓  
TIME 15:27

### --- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 01/03/09  
HEATERS  
SAMPLE CHAMBER: 49c  
BREATH TUBE: 41c  
BAROMETER: 29.65 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

### PRINTER TEST

! " # \$ % & ' ( ) \* + , - . / 0 1 2 3 4 5 6 7 8 9 : ; ( = ) ? @ A B C D E F G  
H I J K L M N O P Q R S T U V W X Y Z [ \ ] ^ \_ ` a b c d e f g h i j k l m n o  
p q r s t u v w x y z { | } ~