

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130526
Name		Joseph V. SHOEMAKER	ID# 4188 Date <del>12-5-07</del> 3/7/2008
A	Agency	SDPI/SAND Point P.D.	Phone # 907-383-3700
Instrument Location		SAND POINT, ALASKA 99661	
Alco S/N		77621	Target Value .084 High Pressure 975
B	Alco Test Value Average	.079	.079
		1 <sup>st</sup> Alco	2 <sup>nd</sup> Alco
Signature		Joseph V. Shoemaker	CSB 3/11/08

(OVER)


(Do Not write in the area below)

Under the Alaska Rules of Evidence, I certify that;

(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Joseph V Shoemaker, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

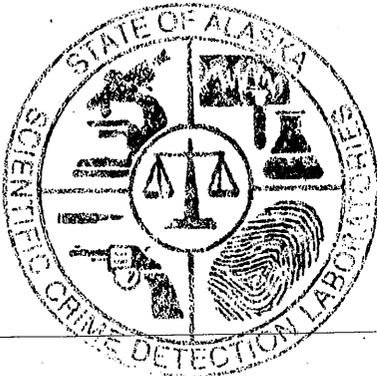

Signed and sealed,

*Jeanne Swartz*

Jeanne Swartz  
Scientific Director Designee  
State of Alaska  
State Breath Alcohol Testing Program

3/12/08  
Date

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N

13 0526

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130526

MARCH 07, 2008

OPERATOR'S NAME:

SHOEMAKER J V

OPERATOR'S NUMBER: 4188

SUBJECT'S LAST NAME:

VERIFICATION OF CAL

SUBJECT'S FIRST NAME/MI :

K

O.L. #: K

DEPT/AGENCY: SDP1

CASE/REPORT: K

TEST TYPE: V

ALCO TARGET VALUE: .084

ALCO S/N: 77621

--- BREATH ANALYSIS ---

.084 ADJUSTED FOR 29.33 in  
ALCO TARGET .082 16:00  
BLANK TEST .000 16:01  
INTERNAL STANDARD VERIFIED 16:01  
ALCO TV 29.34 in .079 16:01  
BLANK TEST .000 16:02  
SUBJECT SAMPLE .000 16:03  
BLANK TEST .000 16:04  
ALCO TV 29.34 in .079 16:04  
BLANK TEST .000 16:05

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130526

MARCH 07, 2008

TIME 16:07

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 02/20/01

HEATERS

SAMPLE CHAMBER: 49c

BREATH TUBE: 42c

BAROMETER: 29.34 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!@#%&'()\*+,-./0123456789:;<=>?@ABCDEF  
HIJ.KLMNOPQRSTUVWXYZ\]^\_`abcde fghijklmnop  
qrs=tuvwxyz{|}~\*