

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130526 ✓
A	Name	Joseph V. SHOEMAKER ID#	4/88 Date 12-5-08
	Agency	SDPI (Sand Point P.D.)	Phone # 907-383-3700
	Instrument Location	SAND POINT, AK 99661	✓
B	Alco S/N	77621 ✓	Target Value .084 ✓ High Pressure 800
	Alco Test Value Average	.079 ✓	.079 ✓
		1 st Alco	2 nd Alco
	Signature	Joseph V. Shoemaker ✓	CAB 12/10/08
(OVER)			


Under the Alaska Rules of Evidence, I certify that, (Do Not write in the area below)

(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Joseph V Shoemaker, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed,

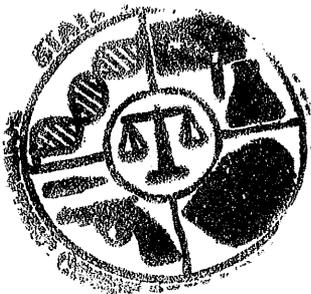

Jeanne Swartz 12/10/08
Jeanne Swartz Date
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N

130526

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130526

DECEMBER 05, 2008

OPERATOR'S NAME:

SHOENAKER J V

OPERATOR'S NUMBER: 4190

SUBJECT'S LAST NAME:

VERIFICATION OF:

SUBJECT'S FIRST NAME/MI:

L

O.L. #: L

DEPT/AGENCY: SDPI

CASE/REPORT: J

TEST TYPE: V

ALCO TARGET VALUE: .004

ALCO S/N: 77621

--- BREATH ANALYSIS ---

.004 ADJUSTED FOR 29.47 in
ALCO TARGET .002 10:12
BLANK TEST .000 10:13
INTERNAL STANDARD VERIFIED 10:13
ALCO TV 29.47 in .079 10:13
BLANK TEST .000 10:14
SUBJECT SAMPLE .000 10:15
BLANK TEST .000 10:16
ALCO TV 29.47 in .079 10:16
BLANK TEST .000 10:17

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130526

DECEMBER 05, 2008

TIME 10:18

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 02/20/01

HEATERS

SAMPLE CHAMBER: 43c

BREATH TUBE: 41c

BAROMETER: 29.47 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!"#\$%&'()*+,-./0123456789:;<=>?@ABCDEFGHIJ
KLMNOPQRSTUVWXYZ[\]^_`abcdefg hijklmno
pqrstuvwxy z{|}~"