

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure: DataMaster cdm S/N 130567

Name Derek A. McGarrigan ID# 025 <sup>5420</sup> Date 3/1/08

A Agency KETCHIKAN POLICE DEPARTMENT ✓ Phone # 225-6631

Instrument Location Ketchikan Police Dept. 361 Main St. Ketchikan, AK 99901

B Alco S/N 65859 ✓ Target Value .081 ✓ High Pressure 1150

Alco Test Value Average .083 .084  
1<sup>st</sup> Alco 2<sup>nd</sup> Alco

Signature [Signature] CRB 3/6/08


(OVER)

(Do Not write in the area below)  
Under the Alaska Rules of Evidence, I certify that,

(a) I am Jeanne Swartz, Criminalist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Derek McGarrigan, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

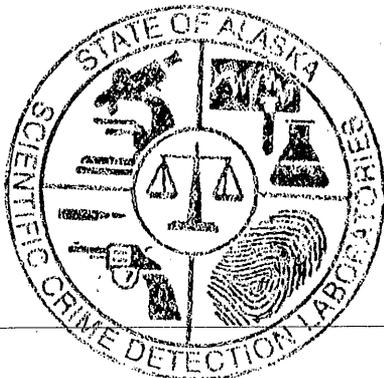

Signed and sealed,

[Signature] 3/7/08  
Date  
Jeanne Swartz  
Scientific Director Designee  
State of Alaska  
State Breath Alcohol Testing Program

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130567

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130567

MARCH 01, 2008

OPERATOR'S NAME:

MCARRIGAN DEREK A

OPERATOR'S NUMBER: 5420

SUBJECT'S LAST NAME:

VOC

SUBJECT'S FIRST NAME/MI:

VOC

O.L. #: 1234567

DEPT/AGENCY: KET1

CASE/REPORT: 00-111

TEST TYPE: V

ALCO TARGET VALUE: .001

ALCO S/N: 65859

--- BREATH ANALYSIS ---

.001 ADJUSTED FOR 29.85 in		
ALCO TARGET	.000	07:30
BLANK TEST	.000	07:31
INTERNAL STANDARD	VERIFIED	07:31
ALCO TV 29.85 in	.003	07:31
BLANK TEST	.000	07:32
SUBJECT SAMPLE	.000	07:33
BLANK TEST	.000	07:34
ALCO TV 29.85 in	.004	07:34
BLANK TEST	.000	07:35

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130567

MARCH 01, 2008

TIME 07:24

--- DIAGNOSTIC CHECK ---

COMPUTER:	OKAY
PROGRAM:	OKAY
SOFTWARE DATE:	02/20/01
HEATERS	
SAMPLE CHAMBER:	50c
BREATH TUBE:	42c
BAROMETER:	29.83 in
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

PRINTER TEST

! " # \$ % ' ( ) \* + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G  
H I J K L M N O P Q R S T U V W X Y Z [ \ ] ^ \_ ` a b c d e f g h i j k l m n o  
p q r s t u v w x y z { | } ~